


# NX

## Key User Manual

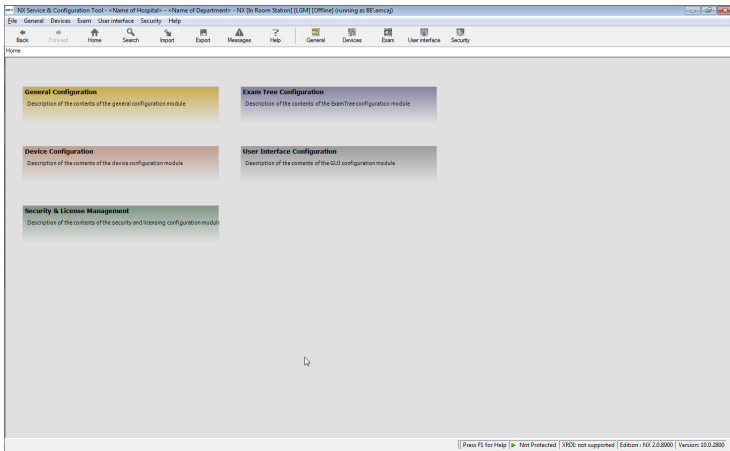

# Contents

Introduction to this Manual .....	6
Scope of this Manual .....	7
About the safety notices in this document .....	8
Disclaimer .....	9
Introduction to NX Service and Configuration Tool .....	10
Intended Use .....	11
Intended User .....	12
Safety Directions .....	13
Using the NX Service and Configuration Tool .....	15
About NX Service and Configuration Tool Versions .....	16
Prerequisites .....	17
Licenses .....	18
Starting the NX Service and Configuration Tool .....	19
Closing the NX Service and Configuration Tool .....	21
Using the File Menu .....	23
Loading the Active Configuration .....	24
Loading a Configuration from File .....	25
Loading a Partial Configuration from File .....	26
Saving a Configuration .....	30
Activating a Configuration .....	31
Verifying a Configuration .....	33
Restoring a Previous Configuration .....	34
Showing Configuration Messages .....	35
The Workspace .....	36
General Configuration .....	37
General Settings .....	38
Site Settings .....	39
Workstation Settings .....	40
Regional Settings .....	43
Predefined Lists .....	46
Custom Markers .....	48
Veterinary Settings .....	50
Mammo Codes Settings .....	51
Workflow Management .....	51
Identification .....	52
Image Presentation .....	58
Emergency Procedure .....	61
Configuring the Devices Connected to NX .....	62
Configuring Archives .....	63
Configuring the List of Archives .....	64
Modifying Archive Properties .....	67
Configuring Digitizers .....	72
Introduction .....	73
Configuring Digitizers System Wide .....	75

Digitizer Settings .....	77
Configuring Export Destinations .....	79
Configuring System Wide Export Destination Settings .....	81
Modifying the Properties of DICOM Export Destinations .....	85
Configuring ID Tablet .....	88
Configuring ID Tablet System Wide .....	89
Configuring Properties of ID Tablet .....	90
Configuring Monitors .....	91
Configuring Printers .....	92
Configuring System Wide Printing .....	93
Modifying the Properties of Existing Printers (Changing Printer Profiles) .....	100
Configuring Priors .....	106
Configuring RIS .....	108
Configuring System wide RIS settings .....	109
Modifying the Properties of Individual RIS .....	110
RIS Mapping .....	115
Configuring the X-Ray Device .....	127
Configuring an X-Ray Device .....	128
Configuring a DR Detector .....	129
Configuring the Generator Settings .....	130
Configuring the Retrofit Box Settings .....	131
Configuring the DR Image Recovery Exposure Type .....	132
Configuring the Room Settings .....	133
Configuring Rooms .....	134
General .....	135
Configuring Workstations for Central Administration .....	137
Configuring Security Issues .....	138
General Security Settings .....	139
Configuring SSL Settings .....	140
Configuring Audit Log Settings .....	140
Managing Users .....	141
General .....	142
Assigning User Roles .....	143
Managing Licenses .....	143
Managing Licenses in the License Manager ....	144
Managing Licenses in the NX Service and Configuration Tool .....	145
Trial Licenses .....	146
Service Log In .....	146
Deleting Examinations .....	147
Configuring the Examination Tree .....	148
Main Window .....	149
Introduction .....	150
Main Screen Functions .....	152

Partial Loading of an Exam Tree .....	156
Tips & Tricks .....	157
Configuring Examination Groups .....	160
Configuring Exposure Types .....	162
General Settings .....	163
Exposure Settings .....	166
Processing and Routing .....	169
Modality Settings .....	175
Configuring Exposure Groups .....	184
Exposure Groups .....	185
Creating Exposure Groups .....	188
Editing Exposure Groups .....	190
Managing Protocol Codes .....	194
Importing Protocol Codes .....	195
Linking Protocol Codes .....	195
Adding new Protocol Codes .....	198
Editing Protocol Codes .....	199
Removing Protocol Codes .....	201
Unassigning Protocol Codes .....	202
Adding Unknown Protocol Codes .....	203
Exporting Protocol Codes .....	204
Configuring the User Interface .....	205
General Settings .....	206
Person Name Configuration .....	207
Image Overview .....	209
Current Patient Switch .....	210
Configuring External Applications .....	212
Worklist Settings .....	213
General Settings .....	214
Worklist .....	218
Closed Exams .....	220
Search .....	222
Examination Settings .....	224
General Settings .....	225
XRG Parameters .....	227
View Patient .....	230
Edit Patient .....	231
View Image Details .....	233
Edit Image Details .....	234
Compose Exam .....	237
Tools & Annotations .....	239
Editing Settings .....	239
General Settings .....	241
Softcopy & Print View .....	243
Tools & Annotations .....	246
Using the Offline NX Service and Configuration Tool .....	258
Introduction .....	259
Prerequisites .....	260
Limitations .....	261
Licenses .....	262

Using the offline NX Service and Configuration Tool	....
263	
Special: Configuring Bitmap Images to be Printed on Film	
.....	265

# Introduction to this Manual

---

## Topics:

- *Scope of this Manual*
- *About the safety notices in this document*
- *Disclaimer*

## **Scope of this Manual**

---

This manual contains information for the safe and effective operation of NX key user tasks and the usage of the NX Service and Configuration Tool.

## About the safety notices in this document

---

The following samples show how warnings, cautions, instructions and notes appear in this document. The text explains their intended use.



**DANGER:**

A danger safety notice indicates a hazardous situation of direct, immediate danger for a potential serious injury to a user, engineer, patient or any other person.



**WARNING:**

A warning safety notice indicates a hazardous situation which can lead to a potential serious injury to a user, engineer, patient or any other person.



**CAUTION:**

A caution safety notice indicates a hazardous situation which can lead to a potential minor injury to a user, engineer, patient or any other person.



An instruction is a direction which, if it is not followed, can cause damage to the equipment described in this manual or any other equipment or goods and can cause environmental pollution.



A prohibition is a direction which, if it is not followed, can cause damage to the equipment described in this manual or any other equipment or goods and can cause environmental pollution.



*Note: Notes provide advice and highlight unusual points. A note is not intended as an instruction.*

## Disclaimer

---

Agfa assumes no liability for use of this document if any unauthorized changes to the content or format have been made.

Every care has been taken to ensure the accuracy of the information in this document. However, Agfa assumes no responsibility or liability for errors, inaccuracies, or omissions that may appear in this document.

Agfa reserves the right to change the product without further notice to improve reliability, function or design. This manual is provided without warranty of any kind, implied or expressed, including, but not limited to, the implied warranties of merchantability and fitness for a particular purpose.

In the United States, Federal law restricts this device to sale, distribution and use by, or on order of, a licensed physician.

# Introduction to NX Service and Configuration Tool

---

## Topics:

- *Intended Use*
- *Intended User*
- *Safety Directions*

## Intended Use

---

The NX Service and Configuration Tool is used for configuring NX Workstations.

It provides means to:

- Configure the devices attached to the NX station.
- Configuring examination trees and the sequence in which the examinations and Exposure types can be selected in the NX GUI.
- Configure the functional behavior of the NX workstation.
- Configure the security settings of the NX workstation.
- Restore previous configuration settings.

After installation the NX Service and Configuration Tool can only be accessed by Agfa service and the Key user.

## **Intended User**

---

This manual is written for trained users of Agfa products. Users are considered as the persons who actually handle the equipment as well as the persons having authority over the equipment. Before attempting to work with this equipment, the user must read, understand, note and strictly observe all warnings, cautions and safety markings on the equipment.

The target audience for this manual is the Key user. The Key user is the application specialist of the hospital with a good knowledge of computer networking and examination tree configuration.

In a real-life situation the Key user will use the NX Service and Configuration Tool to modify the basic configuration performed by Agfa service. If help is needed, the user should contact the IT Department of the site or Agfa service.

## Safety Directions

---

**CAUTION:**

Strictly observe all warnings, cautions, notes and safety markings within this document and on the product.

**WARNING:**

Safety is only guaranteed when an Agfa certified field service engineer has installed the product.

**CAUTION:**

All Agfa medical products must be used by trained and qualified personnel.

**WARNING:**

The user is responsible for judging image quality and controlling environmental conditions for diagnostic softcopy or print viewing.

**WARNING:**

A software algorithm error leading to an image processing failure can cause loss of diagnostic information.

**WARNING:**

A configuration error leading to an image processing failure can cause loss of diagnostic information.

**WARNING:**

The user must follow the hospital quality assurance procedures for covering the risks resulting from errors in the image processing

**WARNING:**

Insufficient image quality can be caused by incorrect initialization of the cassette and plate (resulting in a bad plate type), Incorrect change of default image processing parameters, age group or modality settings, sending images to a not supported printer.

**CAUTION:**

To avoid images being lost due to a power failure, the workstation and the Digitizer have to be connected to uninterruptable power supply (UPS) or an institutional standby

generator. In case of a power failure, the UPS will allow to finalize exposed images that are being scanned.



*Note: Do not position the NX Service and Configuration Tool workstation so that it is difficult to disconnect the mains power connection.*



**WARNING:**

**The following actions may lead to serious risk of injury and damage to the equipment as well as making the warranty void:**

Changes, additions or maintenance to the Agfa products carried out by persons without appropriate qualifications and training.

Using unapproved spare parts



**WARNING:**

Improper changes, additions, maintenance or repair of the equipment or the software can lead to personal injury, electrical shock and damage to the equipment. Safety is only guaranteed when changes, additions, maintenance or repairs are carried out by an Agfa certified field service engineer. A non certified engineer performing a modification or service intervention on a medical device, acts on his own responsibility and makes the warranty void.



*Note: Incorrect IPCtrl values on the tag ExpDose can cause ghost images on the cassette.*



*Note: Every reasonable precaution has been taken during the manufacturing of NX to safeguard the health and safety of persons who will operate this system. Cautions, warnings and notes must be observed at all times.*

# Using the NX Service and Configuration Tool

---

## Topics:

- *About NX Service and Configuration Tool Versions*
- *Prerequisites*
- *Licenses*
- *Starting the NX Service and Configuration Tool*
- *Closing the NX Service and Configuration Tool*
- *Using the File Menu*
- *The Workspace*

## About NX Service and Configuration Tool Versions

---

The NX Service and Configuration Tool has different versions:

<p>“Inroom” online NX Service and Configuration Tool</p>	<p>To be used to configure an in-room NX. Runs on NX itself.</p>
<p>CMS online NX Service and Configuration Tool</p>	<p>To be used to configure a CMS NX. Runs on the CMS NX itself.</p>
<p>Offline NX Service and Configuration Tool</p>	<p>Runs on a separate (non-NX) PC. Eg. the laptop of a Service Engineer. This version is used to prepare an (online) configuration.</p> <p>At startup, you must choose whether the NX Service and Configuration Tool must run in In-room mode or CMS mode (to create a configuration for an in-room or a CMS NX).</p> <p>The manual describes the inroom online version of the NX Service and Configuration Tool.</p>

### Related Links

[Using the Offline NX Service and Configuration Tool](#) on page 258

## Prerequisites

---

- The user needs local administrator rights to load/save/activate the online NX Service and Configuration Tool, independent of the role assigned in NX.

## Licenses

---

The NX Service and Configuration Tool requires licenses available on the system. Otherwise the tool will not start and an error dialog box is shown at startup (except for the offline NX Service and Configuration Tool).

Enabling and disabling licenses in the NX Service and Configuration Tool has an important impact on the GUI and verification logic of the NX Service and Configuration Tool!

More on licenses: “Managing Licenses” .


### Related Links

[Managing Licenses](#) on page 143

## Starting the NX Service and Configuration Tool

To Start the NX Service and Configuration Tool, click the NX Service and Configuration Tool icon on the desktop.


The Start dialog box appears, with the options listed below.

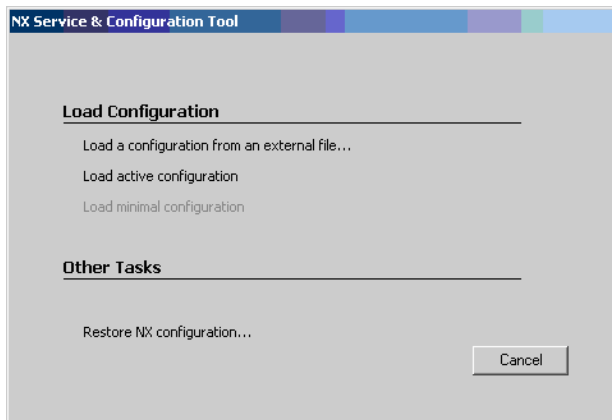

**Figure 1: NX Service and Configuration Tool - Start dialog box**

Load a configuration from an external file	Allows loading a previously exported NX configuration from an xml file (so called 'export file'). Only export files from NX Service and Configuration Tool versions that are equal to or older than current version can be loaded. It is not possible to load a configuration from a newer version of the NX Service and Configuration Tool!  The NX Service and Configuration Tool only allows create a configuration for an NX with the same version!
Load active configuration	Loads the current NX configuration from the NX database to the NX Service and Configuration Tool (makes a copy)
Load minimal configuration	Loads a pre-defined minimal configuration to the NX Service and Configuration Tool. Allowing you to work further on it in order to obtain a complete configuration.
Restore NX configuration	Configuration backups are automatically created by the NX Service and Configuration Tool before activating a new configuration.  With 'Restore NX configuration' it is possible to restore such a previous backup in the NX database.

Clicking on a backup, will display the description entered by the person when doing the activation.

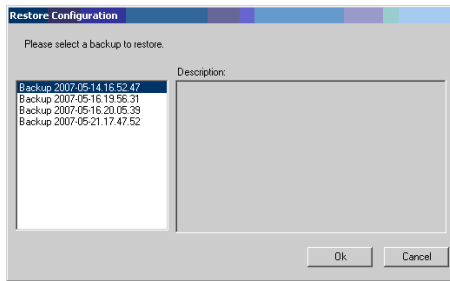


**Figure 2: NX Service and Configuration Tool - Restore dialog box**

These backups are stored in D:\Agfa\Healthcare\NX\Backup\ConfigurationTool

## Closing the NX Service and Configuration Tool

To close the NX Service and Configuration Tool, go to the File menu and select Close.

The Close dialog box appears, with the following options.

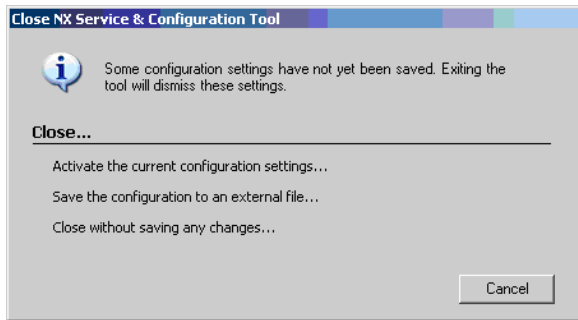

**Figure 3: NX Service and Configuration Tool - Close dialog box**

<p>Activate the current configuration settings</p>	<p>Will load the current configuration (as shown in the NX Service and Configuration Tool screens) in the NX database. First a verification will be done. If errors are detected, the activation will stop. The errors need to be solved first. You will be asked to enter a name and a short description before activation.</p> <p>Prior to the activation, the NX Service and Configuration Tool will create a backup of the current NX database configuration. This backup will be stored in the folder D:\Agfa\Healthcare\NX\Backup\ConfigurationTool. It is possible to restore it later.</p> <p>If the NX Workstation is connected to a Central Monitoring System, the CMS must be restarted to synchronize with the new configuration of the NX Workstation.</p>
<p>Save the configuration to an external file</p>	<p>Allows saving the current configuration work to an xml file. The configuration is not verified. The xml file can later be loaded in the NX Service and Configuration Tool again.</p>
<p>Close without saving any changes</p>	<p>Closes the NX Service and Configuration Tool. All changes will be lost.</p>
<p>Cancel</p>	<p>Closes the Closure dialog box, the NX Service and Configuration Tool is not quit.</p>



*Note: For activating a configuration, a password is required. The password is available to your local Agfa representative and changed on a regular base.*

**Related Links**

[Verifying a Configuration](#) on page 33

## Using the File Menu


---

### Topics:

- *Loading the Active Configuration*
- *Loading a Configuration from File*
- *Loading a Partial Configuration from File*
- *Saving a Configuration*
- *Activating a Configuration*
- *Verifying a Configuration*
- *Restoring a Previous Configuration*
- *Showing Configuration Messages*


## Loading the Active Configuration

When starting up the NX Service and Configuration Tool, the user can choose to load a temporary copy (snapshot) of the NX database in the Workspace via File > Load active configuration:

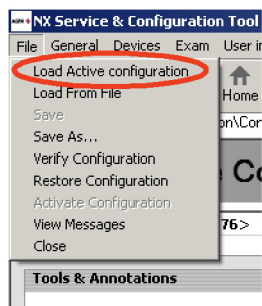

**Figure 4: NX Service and Configuration Tool - File Menu**

He may then work on this temporary copy. Once all modifications have been completed, he can store all the modifications in one transaction to the NX database on the system (via Activate Configuration):



**Figure 5: NX Service and Configuration Tool - File Menu**

This will prevent intermediate and/or unverified modifications of configuration settings ending up in the NX database.

Adapting the configuration in the workspace is risky as there is no auto save of modifications. Finish adaptations to the configuration in one session and then store modifications to the database.

## **Loading a Configuration from File**


Loads a configuration from an external file.

## Loading a Partial Configuration from File

Via the menu 'File – Partial load from file' it is possible to import a part of the configuration.

This allows configuration replication between NX systems that share common settings.

Existing settings will be overwritten!

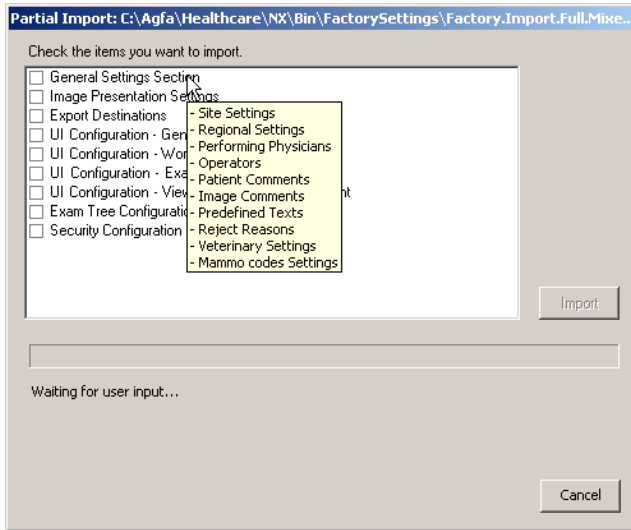

**Figure 6: NX Service and Configuration Tool - Partial Import dialog box**

When hovering over an item, its content is displayed.

The items that can be imported selectively are listed below. Upon import of an item (e.g. General Settings) all sub-items contained within the item are imported along (i.c. Site settings, Performing physicians list, etc.):

Item	Contains	In-room	Central
General Settings Section			
	Site settings	X	X
	Regional settings	X	X
	Performing physicians	X	X
	Operators	X	X
	Patient Comments	X	X

Item	Contains	In-room	Central
	Image comments	X	X
	Predefined texts	X	X
	Reject reasons	X	X
	Veterinary settings	X	X
	Mammo codes settings	X	X
Image Presentation Settings			
	Burn	X	O
	Square marker	X	O
	Transparent Shutters	X	X
	Font size	X	X
	Collimation Border Density	X	O
Export Destinations			
	Export Destinations	X	X
UI Configuration – General Settings			
	General Settings	X	X
	- Person Name Composition	X	X
	- Person Name Representation	X	X
	Image Overview Pane	X	X
	Current Patient Switch	X	X
	Configure External Applications	X	X
UI Configuration – Worklist Environment Settings			
	General settings	X	X
	Configure worklist	X	O
	Configure closed list	X	O
	Configure search pane	O	X
UI Configuration – Examination Environment Settings			

Item	Contains	In-room	Central
	General settings	X	X
	Configure XRG parameters	X	X
	Configure view patient pane	X	X
	Configure edit patient pane	X	X
	Configure view image detail pane	X	X
	Configure edit image detail pane	X	X
	Configure tools in examination	X	X
	Custom markers	X	X
UI Configuration – Viewing & Editing Environment Settings			
	General settings	X	X
	Configure normal mode & print mode	X	X
	Configure Tools & Annotations	X	X
	Show true scale factor (Print View)	X	X
Exam Tree Configuration			
	Complete exam tree /w all age groups	X	O
	Add Image Pane configuration	X	O
	NX Emergency settings	X	O
	Exposure groups	X	O
	Protocol codes	X	O
	Print sheets	X	O
Security Configuration			
	General Settings:	X	X
	- Configure SSL settings	X	O
	- Configure audit log settings	X	X
X= imported; O = not imported			



*Note: Upon import of these items, already defined values will be overwritten.*

## Importing exam tree settings from system with different X-ray device

1. If all settings must be imported, start by loading the configuration from file.
2. Delete the x-ray device.  
All modality settings are deleted from the exam tree.
3. Create a new x-ray device and configure the DR Detector(s).
4. Load a partial configuration from the configuration file, selecting the Exam Tree Configuration.

Depending on the version of the installed XRDI software, the imported data is merged with the new device configuration.

After the import, a dialog is displayed with feedback about the import process. If the X-ray modality is found to be incompatible with the imported data, a warning message is displayed that all modality settings are cleared.



*Note:* Alternatively the exam tree settings can be added using the **Add exams** link. The modality settings must be applied manually after the import.

### Related Links

[Loading a Configuration from File](#) on page 25

[Configuring an X-Ray Device](#) on page 128

## **Saving a Configuration**

Saves the current configuration as an external file.

## Activating a Configuration




*Note: For activating a configuration, a password is required. The password is available to your local Agfa representative and changed on a regular base.*

To store the configuration settings in the Workspace to the NX database:

1. Click **File > Activate Configuration**.
2. Enter the password.

The following window appears.

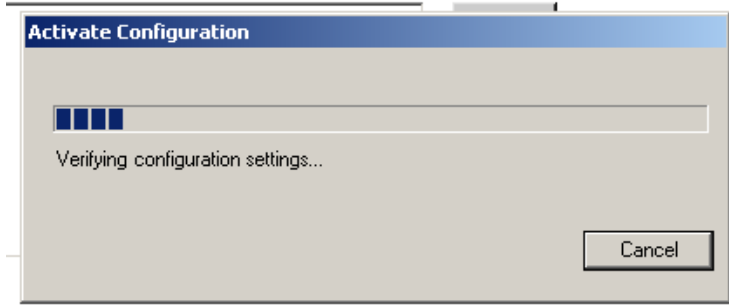


**Figure 7: NX Service and Configuration Tool - Activate Configuration dialog box**



*Note: Changes made to the configuration must be documented in the history list. The key user is forced to comment changes for liability reasons.*

If you activate a configuration, the current configuration is checked (verification).

Following dialog box, with the options listed below, may be shown when errors are detected.

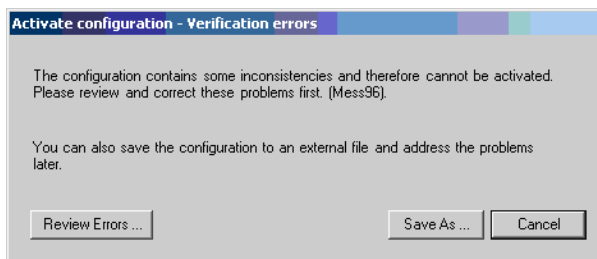

**Figure 8: NX Service and Configuration Tool - Verification Errors dialog box**

Review errors	Brings up all errors and warnings found during verification, The errors must be solved before activation will be possible.
Save as	Allows saving current work to file for later.
Cancel	Closes the verification dialog box

## Verifying a Configuration


It is possible to verify a configuration without activating it. Click file – verify configuration. After the verification, the errors and warnings are shown.

## Restoring a Previous Configuration

To restore a previous configuration of NX

### 1. Select **Restore Configuration**.

The system lists all the available backups and asks the user to select the required backup:

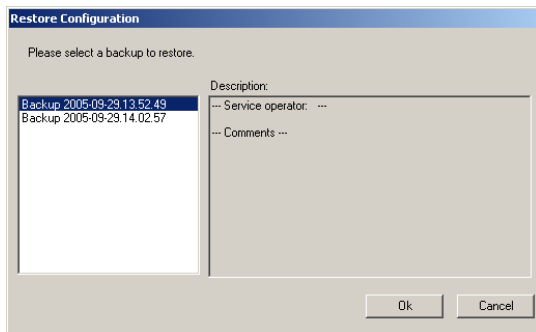

**Figure 9: NX Service and Configuration Tool - Restore Configuration dialog box**

2. Select the backup to restore.
3. Consult the description of the backup file.
4. Click OK.

The system creates a backup of the current set of configuration settings in the NX database.

## **Showing Configuration Messages**

Shows the messages generated by the NX Service and Configuration Tool during the configuration activities.

## The Workspace

---

All main activities in the NX Service and Configuration Tool are performed in the Workspace.

The Workspace is mainly introduced for the purpose of safety and to monitor the consistency of the configuration settings of the NX database. The Workspace creates a safe environment in which you can make any modifications to the configuration settings, test and verify them without affecting the actual configuration settings of NX.

# General Configuration

---

## Topics:

- *General Settings*
- *Workflow Management*

## General Settings

---

### Topics:

- *Site Settings*
- *Workstation Settings*
- *Regional Settings*
- *Predefined Lists*
- *Custom Markers*
- *Veterinary Settings*
- *Mammo Codes Settings*

## Site Settings

### Topics:

- [Hospital Name, Hospital Address, Department Name](#)
- [Performing Physician](#)
- [Operators](#)

### Hospital Name, Hospital Address, Department Name

These site settings are included in the DICOM tags when sent to PACS, MPPS. They can be overruled by the values included in the DICOM modality worklist.

Hospital Name: (0008,0080)

Hospital Address: (0008,0081)

Department name: (0008,1040)

### Performing Physician

The Performing physician names (0008,1050) entered here can be selected in edit patient screen when configured. The maximum number of physicians that can be entered is 50.

Edit Patient		
1	Last Name :	Position: 7
2	First Name	Label: Performing Physician Last Name :
3	Patient Identification	Content: Performing Physician Last Name ;(0008,1
4	Birth Date :	IME:
5	Sex :	<input type="checkbox"/> Is mandatory field
6	Comments :	
7	Performing Physician	
8		

Figure 10: NX Service and Configuration Tool - Edit Patient pane

### Related Links

[Edit Patient](#) on page 231

### Operators

Pre-define a list of operators. The maximum number of operators that can be entered is 50.

The list will be used in NX when the ‘Force operator identification...’ flag is enabled (see “Identification”):


Operator Name \_\_\_\_\_

Force operator identification on start exam

Link user name to operator name

Figure 11: NX Service and Configuration Tool - Operator Name section

In this case, the operator has to identify himself by selecting an operator name the first time one wants to identify an exposure in a new exam in NX:

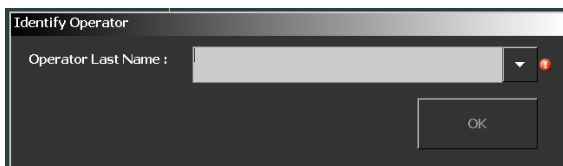

**Figure 12: NX - Identify Operator dialog box**

This list is also used in the “Select a Reject Reason” dialog box.

### Related Links

[Identification](#) on page 52


## Workstation Settings

### Topics:

- [Workstation General Settings](#)
- [Workstation Fast Preview Settings](#)
- [Workstation Fast ID](#)
- [Workstation Storage Commit](#)
- [Workstation Musica Micro Calcification Enhancement Settings](#)

### Workstation General Settings

Field	Description
ID station name	<p>This name is used in the DICOM Digitizer CPF as the identification of the NX for fast ID functionality.</p> <p>Further, this attribute is also set in the station name (0008, 1010) in MPPS or RIS.</p> <p>This is not the station name (0008,1010) attribute used in the C-STORE commands. In C-STORE the station name is set to the Digitizer name.</p>
Performed location	Only here for informational purposes, not used further
Processing station name	<p>NX will write the Processing station name to the cassette. The DICOM Digitizer uses this to determine to which NX station it needs to send the image to. Must not be identical to the hostname of the PC. Fill in a dummy value when a twain Digitizer is connected (as this field is not used then).</p>

Character set	<p>Used for communication with DICOM RIS, MPPS and PACS systems. Not used when communicating with Digitizers.</p> <p>The NX Station will only send out characters which are defined in the selected character sets</p>
<p>Enable automatic cassette identification (also called 'auto-ID')</p>	<p>When enabled: on insertion of the cassette in the ID tablet or Digitizer, the cassette is automatically identified with the exposure settings selected at that moment in NX.</p> <p>The ID button in NX remains disabled in this setup.</p> <p>Except when the Examination screen is not in front in NX and a cassette is inserted, a dialog pops up telling the user to go to the examination screen. The user must manually press the ID button in that case (which is then enabled)!</p>  <p><b>Figure 13: NX - Identify Cassette error dialog box</b></p> <p>If the selected exposure has already been exposed, a copy of it is made when a cassette is inserted.</p> <p>To obtain this functionality with a Digitizer, the Fast ID flag must be enabled in the Digitizer setup and configured further. Otherwise auto-ID will not work. Also the Digitizer has to support this feature.</p>
Performed station AE title	<p>The AE title to be used for all SCU's of the NX station (MPPS, Archiving etc.) and for the storage SCP from the Digitizer (NX as SCP).</p>
Show IP addresses (button)	<p>Click the button to view the IP addresses (IPv4 or IPv6) of the NX on the local network, used to connect to DICOM digitizers, RIS, PACS, etc. The IP address is automatically detected at time of last start-up of the NX Workstation.</p>

port	The port number for receiving the images from the Digitizer (NX as SCP).
Default modality	Modality type to be used as default setting for creating a new RIS device or configuring MPPS.

### Related Links

[CPF Generation](#) on page 78

[Workstation Fast ID](#) on page 42

## Workstation Fast Preview Settings

Settings only used with DICOM Digitizers (but still these fields need to be filled in for Twain Digitizers too).

Field	Description
AE title	The NX AE title for receiving fast preview images from Digitizer (NX as SCP)
Port number	The NX port number for receiving the fast preview images

## Workstation Fast ID

(fast ID is sometimes also called 'direct ID')

Field	Description
Enable fast ID	To be enabled when no ID tablet is used. Identification happens on the Digitizer.  Only supported with non-buffered Digitizers (DX-S, CR30, Solo). Mandatory with DX-S and CR30.  Pressing the ID button (Identification) can be done before or after insertion of the cassette in the Digitizer.  Fast ID needs also to be configured in the Digitizer.
AE title	The AE title on NX to which the Digitizer sends the fixed cassette info. (not needed for Twain Digitizer, fill in dummy value)
Port number	The AE title on NX to which the Digitizer sends the fixed cassette info.  (Not needed for Twain Digitizer, fill in dummy value.)

### Related Links

[Digitizer Settings General](#) on page 77

## Workstation Storage Commit

Field	Description
Enable storage commit	<p>With storage commit, the archive reports back to NX when the archive job is successfully archived.</p> <p>Archive storage commit AE title and port need to be configured in the archive settings.</p> <p>NX will open an association to request storage commit to the archive. The archive opens an association back to NX to confirm storage commit. This is the only DICOM scenario where an SCP (the archive) starts an association.</p>
AE title	The AE Title for receiving the storage commit result message (NX as SCU).
Port number	Port number on which NX receives storage commit communication from archive.
Enable SSL	Whether the storage commit communication should be done securely (requires SSL certificates)

### Related Links

[Storage Commit](#) on page 71

## Workstation Musica Micro Calcification Enhancement Settings


Field	Description
AE title Port number	AE title and Port number for receiving processed images from the Micro Calcification Enhancement (MCE) Engine. In most situations the default values should not be changed.

## Regional Settings

### Topics:

- [Regional Settings General](#)
- [Regional Settings and CMS](#)

## Regional Settings General

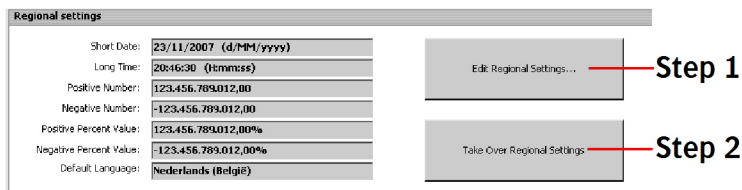

**Figure 14: NX Service and Configuration Tool - Regional Settings**

Allows changing some regional settings for nx.

These settings apply for all users using nx. they are user independent.

Most important settings are the date and time formats.


Set the default language to the language most likely to be used in the customer's environment.

- Step 1

Edit regional settings by clicking the 'edit regional settings' button. this brings up the windows regional and language options dialog.

To change the time and date format, click the additional settings button on windows 7 or the customize button on windows xp.

Pressing ok twice will save these settings in windows.

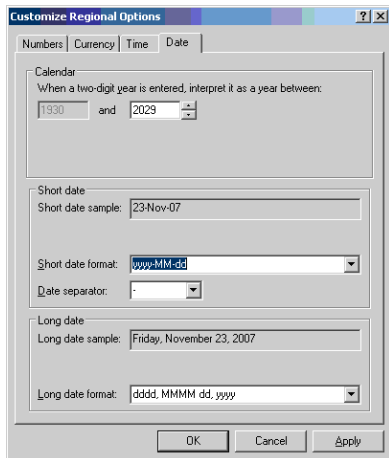

**Figure 15: Windows - Regional Settings**

- Step 2:

Pressing the 'Take over Regional settings' button in the NX Service and Configuration Tool will copy the settings (only those that are listed in the NX

Service and Configuration Tool – see screenshot above) to the NX database after activation.



*Note: Any user can configure the Regional Settings in Windows and the NX Service and Configuration Tool. This is not restricted to certain user roles.*

It is now guaranteed that the date and time formats of NX are the same as the date and time settings configured in the Windows Regional Settings. If, for example, “date” in Windows is formatted as “day/month/year” and this setting is taken over in NX, a possibly confusing date as 3/6/2007 cannot have a different meaning in Windows and NX.

**Figure 16: NX - Edit Patient pane**



*Note: Previous versions of NX required the “Change backend user locale” script to be run. From NX 3.0 on, this is not longer required.*



*Note: Above settings have no relation to the language(s) to be used in NX.*

## Regional Settings and CMS



Even on CMS, Regional Settings can be configured.


It is strongly advised to make sure all settings are the same in an NX cluster (several NX workstations connected to a CMS).

In an NX cluster, the CMS will issue a warning at startup when it detects that regional settings are conflicting.

“Conflicting regional settings detected. Please verify configuration of in-room station(s)...”

## Predefined Lists
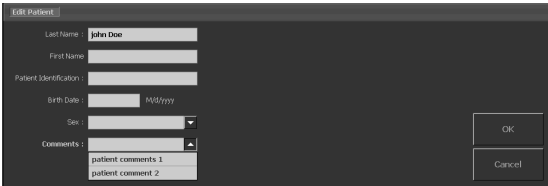
<p>Patient comments</p>	<p>Patient comments can be edited here.</p> <p>They are used in the Edit Patient screen.</p>  <p><b>Figure 17: NX - Patient Comments section</b></p> <p>The visibility of patient comments also needs to be activated in the 'Edit Patient' setup screen.</p>
<p>Predefined texts</p>	<p>Predefined texts can be edited. They are used in the Examination screen.</p>  <p><b>Figure 18: NX - Predefined texts</b></p> <p>Each predefined text can have a different font size.</p>
<p>Image comments</p>	<p>Image comments can be edited</p> <p>The visibility of image comments also needs to be activated in the Edit Image Details setup screen.</p>

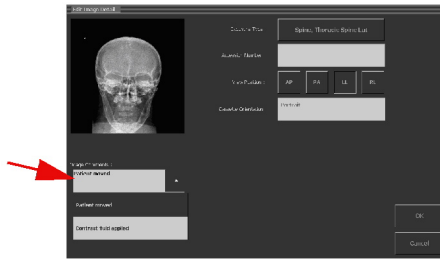

**Figure 19: NX - Image Comments**

Custom Fields	<p>Up to five custom editable fields can be configured to be added to the patient data or to the image data.</p> <p>The visibility of custom fields also needs to be activated in the Edit Patient setup screen or the Edit Image Details setup screen.</p>
---------------	---

### Related Links

[Edit Image Details](#) on page 234

[Edit Patient](#) on page 231

## Custom Markers

It is possible to define custom markers here, apart from predefined fixed markers such as Left and Right



*Note: Also refer to the image laterality item under Exposure Settings for General Radiology Examinations in the exam tree.*

The screenshot shows the 'Exposure Settings' dialog box. It contains several fields and options:

- Body Part:** Chest
- Anatomic Region:** Chest
- View Code:** left: lateral
- Auto-flip lateral images:**
- View Position:**
  - AP
  - PA
  - LL
  - RL
- Automatically update image laterality when adding marker:**  (highlighted with a red box)
- Image Laterality:**
  - Left
  - Right
  - Both
  - Unpaired

**Figure 20: NX Service and Configuration Tool - Exposure Settings pane**

Another fixed marker is the High Priority Marker (HPM). It can be used to indicate to a radiologist that something of interest was seen on this image. Adding the high priority marker to an image will also increase the study priority ID to medium. This will assist your PACS system to identify these exams and handle them in an appropriate way.

After adding a new marker, its visibility must be configured in User Interface Configuration.

**Step 1 :**  
 Add a custom marker to  
 the NX database.

Custom markers

Name	Text	Functionality	Size
L	L	Left	10
R	R	Right	10
HPM	*	High priority	10
SIT	Patient sitting		10
DOWN	Patient laying down		10
STAND	Patient standing		10
My	my marker		10
	[add a new marker]		
	[add a new marker]		
	[add a new marker]		
	[add a new marker]		
	[add a new marker]		

**Step 2:**  
 Configure the NX User  
 Interface for the marker.

User Interface Configuration

General Settings

XRG Parameters

View Patient

Edit Patient

View Image Details

Edit Image Details

Compose Exam

Tools & Annotations

1 2 3 4 5

L R ←→ ↻ ↺

6 7 8 9 10

STAND DOWN My

Content: Left Marker

**Result:**  
 The marker appears in  
 NX.

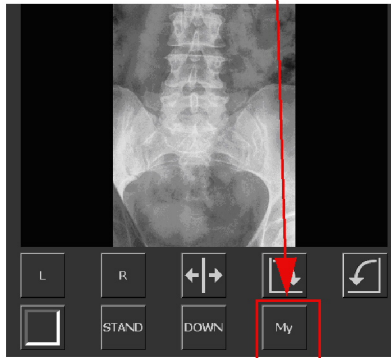


Figure 21: Adding Custom Markers - Overview

Related Links

[Annotations Palette](#) on page 247

## Veterinary Settings

Species Name	Contains the value for DICOM attribute (0010,2201)
Breed Name	Contains the value for DICOM attribute (0010,2292)
Breed Registration Number	Contains the value for DICOM attribute (0010,2295)
Breed Registry Code Sequence	Contains the value for DICOM attribute (0010,2296)
Responsible Person	Contains the value for DICOM attribute (0010,2297)
Responsible Person Role	Contains the value for DICOM attribute (0010,2298)
Responsible Organization	Contains the value for DICOM attribute (0010,2299)
Patient's Sex Neutered	Contains the value for DICOM attribute (0010,2203)

These field scan be made visible and/or editable in the UI configuration.

### Related Links

[View Patient](#) on page 230

[Edit Patient](#) on page 231

## Mammo Codes Settings

It is possible to change the names (Eg. translate) of the View modifier values (0054, 0222) and Requested Procedure Reason values (0040, 100A).

These attributes can be made visible in the View/Edit image details pane.

Code	Specifies the code
Meaning	Specifies the default meaning of the code
Text	Contains the customizable text for the selected code. This is the text string that will be used to display the attribute in the View/Edit image details pane when made visible.
Revert	Resets the (customized) values of the “Text” attributes to the values of the “Meaning” attribute.

### Related Links

[View Image Details](#) on page 233

[Edit Image Details](#) on page 234

## Workflow Management

---

### Topics:



- [Identification](#)
- [Image Presentation](#)
- [Emergency Procedure](#)

## Identification

### Topics:

- *Identification General*
- *Storage*


### Identification General
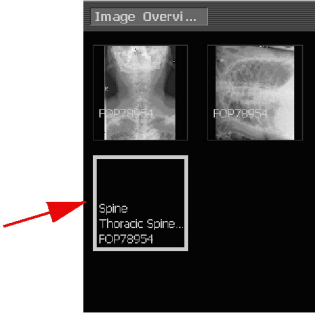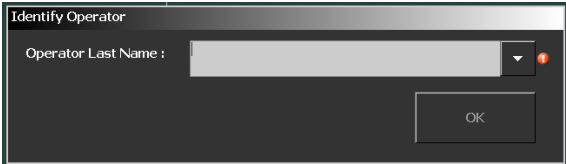
<p>Automatic selection of next exposure thumbnail</p>	<p>Defines whether the next exposure thumbnail in the NX image overview pane will be automatically selected after identification.</p>  <p><b>Figure 22: NX - Automatic Selection of Next Image Thumbnail</b></p> <p>When xrg license is enabled, this will not work.</p>
<p>Force operator identification on start exam</p>	<p>When enabled, the operator has to identify himself by selecting (or entering) an operator name the first time he wants to identify an exposure in a new exam in nx:</p>  <p><b>Figure 23: nx - Identify Operator Dialog Box</b></p> <p>and in the reject reason dialog:</p>



**Figure 24: NX - Select Reject Reason Dialog box**


An operator name can be typed-in or a pre-defined list of operators can be configured in General Configuration – Site Settings:

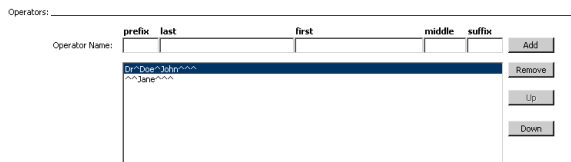


**Figure 25: Nx Service and Configuration Tool - Operator List Section**

The operator name (0008, 1070) is also used in audit logging.

<p>Link user name to operator name</p>	<p>When enabled, the name of the user logged in (on Windows) is used as operator name (0008, 1070). This operator name is also used in audit logging.</p>
<p>Lock RIS patient demographics</p>	<p>Selecting this will prevent editing of patient data sent by the RIS. Manually created exams can still be edited.</p> <p>This prevents inconsistencies with the RIS system. This is the default IHE behavior.</p>

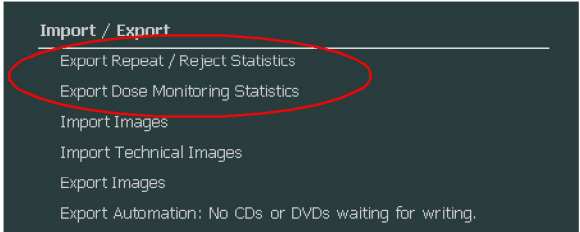	<p>If MPPS is configured, editing of patient data will always be prevented on data, independent of this setting after first image arrival.</p>
<p>Lock patient demographics when archiving images</p>	<p>Selecting this will prevent editing of patient data, but only after the first image is sent to PACS. Applies to patient data coming from RIS and manually created exams.</p> <p>If MPPS is configured , editing of patient data will always be prevented on data, independent of this setting after first image arrival.</p>
<p>Days to keep exams on the system</p>	<p>Defines the maximum number of days a closed exam is stored within the history list. Don't set it any higher than really needed because it will impact system performance.</p>
<p>Store dose and RRAP statistics centrally</p>	<p>Enable this check box if you want to manage dose and RRAP (Repeat\Reject) statistics centrally (on CMS).</p> <p>The CMS will periodically collect these statistics from the in-room NX and buffer them. At that moment, the list with records on in-room is cleared.</p> <p>If you have selected this option, the main menu options <b>Export Repeat Reject statistics</b> and <b>Export Dose monitoring statistics</b> will be disabled on the in-room NX. Exporting these statistics must be done on CMS then.</p>  <p><b>Figure 26: NX Main Menu - Import/Export section</b></p> <p>On CMS this setting is indicated for every connected in-room NX in the scan result dialog:</p>

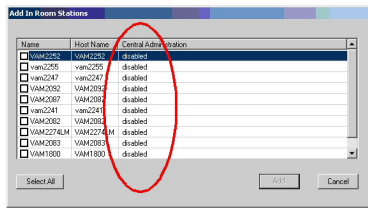


**Figure 27: NX Service and Configuration Tool - Add In Room Stations**

It is advised to set this the same for all in-room NX workstations connected to CMS.

Reject Archive

Defines the reject archive. The reject archive stores rejected images.

Needs to be setup in the archive main pane:




**Figure 28: NX Service and Configuration Tool - Reject Archive**

RRAP Maxlength

Maximum number of RRAP (Repeat\Reject) records that will be kept on this NX. This field is not editable (just shown for information).


When this maximum number is reached, the oldest records will be removed from the database (FIFO).

When the user exports the Repeat\Reject statistics to file (see Main Menu of NX), all records are removed from the NX database.

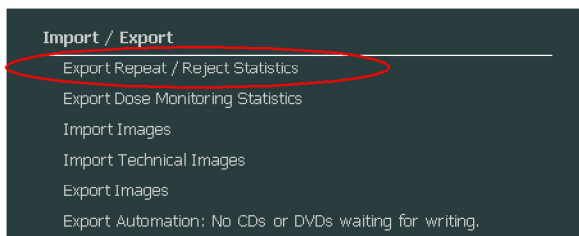

**Figure 29: NX Main Menu - Import/Export section**

In daily situations, this maximum is never reached on the in-room when these statistics are kept centrally as

	the CMS collects them periodically. However be aware that the CMS has a similar maximum!
Request a reject reason  Predefined reject reasons	<p>Activation/deactivation of the request for reject reason. A dialog with these reasons is presented when an image is rejected on NX.</p>  <p><b>Figure 30: NX - Select Reject Reason dialog box</b></p> <p>The list of reject reasons can be configured here.</p>
Enable the <b>Create DR Sequence</b> button	Defines whether the <b>Create DR Sequence</b> button is visible in the NX <b>Add Image</b> pane.

### Related Links

[Configuring Main RIS Settings](#) on page 109

[Storage](#) on page 56

### Storage

NX checks for cleanup of closed exams every hour.

Exams older than the configured number of days are removed (along with their corresponding images).



*Note: Manually re-opening an exam will reset the date of the exam! So it will be cleaned-up later.*

Following exams are not cleaned up (yet):

- Exams which are more recent than 1 day.
- Exams for which archiving or printing failed.
- Exams which are waiting in the DICOM export buffer to be written to CD \DVD (see export automation under “Configuring Export Destinations”).


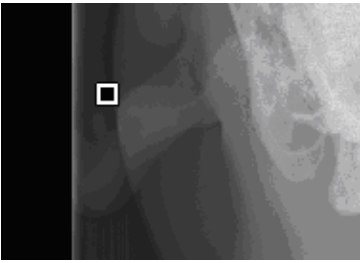



*Note: When there is less than 6Gbyte of free disk space on the image partition (D:), then the oldest exams are cleaned up (even when they are more recent than the ‘days to keep...’ setting).*


#### **Related Links**

[DICOM Export](#) on page 81

## Image Presentation

Enable burn	<p>When enabled: each new received image is displayed 'burned'.</p>  <p><i>Note: In burned images, the pixels that fall outside of the Window (Cfr. Window \Level) are rendered in black or white (depending on which side of the Window they are).</i></p>
Enable ERMF	<p>When enabled: ERMF can be used for new received images:</p> <ul style="list-style-type: none"> <li>• Mammo Magnification factor will be used for measurements and true size calculations (when available)</li> <li>• DR FLFS images are ERMF calibrated (when the patient to grid distance is available)</li> <li>• ERMF calibration button will become available, if it is configured in Annotations Palette and if the SID is known.</li> </ul>
Show Square Marker	<p>When enabled, the square marker is positioned on the image when it arrives on NX. The square marker will be rotated with the image and will trigger the operator or radiologist.</p> <p>Not for mammo images.</p>  <p><b>Figure 31: NX Show Square Marker dialog box</b></p>
Transparent Shutters	<p>When enabled: the shutters are transparent (otherwise shutters are black).</p>

Display mammo images in split screen	<p>Defines whether mammo images should be displayed in split screen view by default.</p>  <p><i>Note: the setting is configured on the in-room NX Workstation. The CMS behaves according to the setting on the selected in-room NX Workstation.</i></p>
Free text Font size	Set font size for free text annotations.
Collimation border density	<p>Value between 0 (lowest density= transparent) and 100 (highest density=black).</p> <p>Auto collimation and the auto display of a black border are configurable per exposure type in the exam tree.</p> <p>If the density is set to 100, collimation borders are transparent. The check box <b>Use non transparent borders for density 100 for Musica 2 and Musica 3</b> makes collimation borders non transparent.</p>
Use non transparent borders for density 100 for Musica 2/3	Collimation borders for Musica 2 and Musica 3 image processing remain transparent, even for density 100. This option forces non transparent collimation borders.
Default DR FLFS Stitching Mode	The selected stitch mode will be used as default for all DR FLFS exams. In the Stitching pane on the NX workstation, the user can switch to the other mode or manually adjust the DR Full Leg Full Spine image.
Show dose deviation	Show/hide dose deviation bar in examination environment.
Max # of records	<p>Maximum number of dose records that will be kept on this NX. This field is not editable (just shown for information).</p> <p>When this maximum number is reached, the oldest records will be removed from the database (FIFO). When the user exports the dose statistics to file (see Main Menu of NX), all records are removed from the NX database.</p>

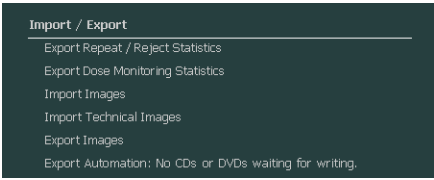	 <p><b>Figure 32: NX Main Menu - Import/Export section</b></p> <p>In daily situations, this maximum is never reached on the in-room when these statistics are kept centrally as the CMS collects them periodically. However be aware that the CMS has a similar maximum!</p>
Musica 2 and Musica 3 Presentation State settings	<p>These fields are used to configure the taste setting belonging to Musica 2 and Musica 3 packages. ‘Taste’ means the combination of contrast, brightness, sharpness and processing version. One has the option to change the taste per package. From then on, this taste is applied to all exposures in that package.</p> <p>The ‘Store’ button just puts the value in the table.</p>
Musica MCE Density	<p>Intensity of the Musica Micro enhancement of the calcifications.</p>

## Emergency Procedure

Here you can configure the settings that NX has to load in a new emergency exam.

Emergency mode	What will be set in the emergency exam.
Empty	Nothing, the new emergency exam created will not have any preconfigured value.
Patient	The configured patient name and ID. NX will add date and time to the name and ID to guarantee uniqueness.
Exposures	The configured Exam or exposure group. This might save a few mouse clicks for the operator when starting an emergency exam on NX.
All	All: The configured patient name, ID and exam or exposure.

# **Configuring the Devices Connected to NX**

## **Topics:**

- *Configuring Archives*
- *Configuring Digitizers*
- *Configuring Export Destinations*
- *Configuring ID Tablet*
- *Configuring Monitors*
- *Configuring Printers*
- *Configuring Priors*
- *Configuring RIS*
- *Configuring the X-Ray Device*
- *Configuring Rooms*

## Configuring Archives

---



*Note: If no automatic archiving, printing or exporting is configured, unrecoverable image loss can happen if an exam is closed before the images are archived, printed or exported, because it may be automatically deleted by the automatic clean up.*

### Topics:


- [\*Configuring the List of Archives\*](#)
- [\*Modifying Archive Properties\*](#)

## Configuring the List of Archives


### Topics:

- [Configuring General](#)
- [Adding a New Archive](#)
- [Configuring Dose Reporting](#)

### Configuring General
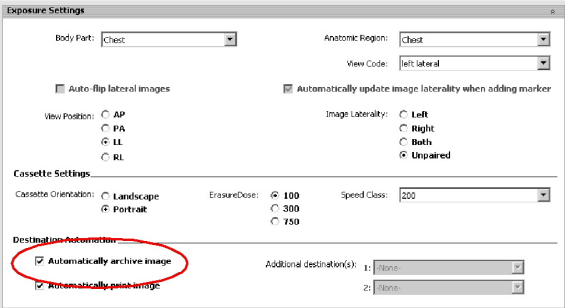
<p>Enable archive automation</p>	<p>If enabled, the configured archive is used to send images to after the <b>Close And Send</b> or <b>Send Image</b> buttons in NX are pressed.</p> <p>If not enabled, no automatic archiving will be done on 'Close and Send'. It is then still possible to archive an image manually by pressing the 'Send Image' button on NX.</p> <p>This setting can be overruled. Per exposure, archive automation can be disabled.</p>  <p><b>Figure 33: NX Service and Configuration Tool - Layout Settings pane</b></p>
<p>Repeat Reject Archive Destination</p>	<p>If enabled, the configured destination will be used as the reject archive destination for rejected images.</p>

## Adding a New Archive

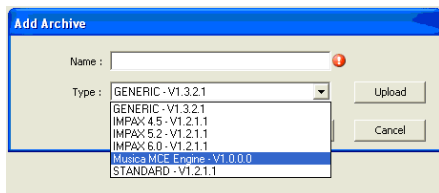

**Figure 34: NX Service and Configuration Tool - Add Archive dialog box**

Press the New button to add a new archive.

- Name: Fill in an nickname for this archive.
- Type: The type field allows you select an archive model. These models contain predefined parameters. After loading, these parameters can be changed per archive.

If the requested archive model is not available on the system, a generic archive model must be selected. The version number (E.g. V1.2.1.0) is just the version number of the model itself.

The Upload button allows you to add a new model or update an existing model. Browse to a proper archive xml file. The model will be added to the NX database for later usage.

If NX is configured to perform Micro Calcification Enhancement (MCE) on mammography images, the images are first sent to a special archive of the type “MCE Engine”. The MCE Engine archive destination does not store the images, but performs the MCE image processing jobs. The processed images are sent back to the NX. Then both the original image and the processed image are submitted for storage on a PACS archive that accepts MCE images.

## Configuring Dose Reporting

NX can create Dose Structured Reports containing information about estimated patient radiation exposure resulting from imaging procedures. The reports can be sent to the archive or to a dedicated Dose Info Reporter or Dose Info Consumer.

Figure 35: Dose Reporting Destinations

## Topics:

- *To configure for sending dose reports to the archive*
- *To configure for sending dose reports to a Dose Information Reporter/Consumer*

### To configure for sending dose reports to the archive

Select each archive and configure these settings:

Support Dose Reporting	Check <b>Support Dose Reporting</b> for the archives to which NX can potentially send dose reports.
AE Title Port Enable SSL	Modify the device settings if the settings for receiving dose reports are different from the settings for receiving images. Click <b>Test Connection</b> to check if the device can be connected (this is not a test to check if the device can receive dose reports).

On 'Close and Send', dose reports are sent to the archive that has Archive Automation enabled and that supports Dose Reporting. The dose reports are processed as separate entries in the archive queue.

If the archive queue is rerouted, the rerouted archive will receive the dose reports, if it is configured to support Dose Reporting.

## To configure for sending dose reports to a Dose Information Reporter/Consumer

Click **Create** and configure these settings:

Name	Nickname for the Dose Information Reporter/Consumer device
Host Name	Enter the device settings.
IP Address	Fill in either hostname and IP Stack or IP address (IP Stack detected automatically).  Click <b>Test Connection</b> to check if the device can be connected (this is not a test to check if the device can receive dose reports).
IP Stack	
AE Title	
Port	
Enable SSL	

On 'Close and Send', dose reports are sent to the configured Dose Information Reporter/Consumer. The dose reports are processed in a separate archive queue.

## Modifying Archive Properties

### Topics:

- [Device Settings](#)
- [Advanced Settings](#)
- [Storage Commit](#)

### Device Settings

Type	The selected model (type)
Hostname	Fill in either hostname and IP Stack or IP address (IP Stack detected automatically).
IP address	
IP Stack	
AE title	DICOM AE title of the archive device for C-STORE (can be in lower case)
DICOM port	Port number of the archive device for the C-STORE  DICOM Store and storage commit can have different port numbers!
Enable SSL	Enable secure DICOM for the C-STORE request, requires SSL Certificates!

Is Archive	if enabled, images sent to this destination will be referenced in the MPPS messages
SOP class	<p>SOP class to be used</p> <p>Combinations of multiple values are possible to allow different output types for GenRad and Mammo images (on mixed user systems):</p> <ul style="list-style-type: none"> <li>• CR For Presentation &amp; MG For Presentation</li> <li>• DX For Presentation &amp; MG For Presentation</li> <li>• DX For Processing &amp; MG For Processing</li> </ul>
GSPS supported	When enabled: the GSPS will be sent together with the image. Otherwise annotations are burned in the image.
Output type	<p>Contents of the list depends on selected SOP class and 'GSPS supported' flag.</p> <p>When using Musica 2 or Musica 3 image processing (Musica 2 or Musica 3 license is active), it is strongly advised to configure for using P-values!</p> <p>Sending Musica 2 or Musica 3-processed images as OD-rel data to the archive will cause insufficient image quality :</p> <ul style="list-style-type: none"> <li>• background showing contouring and artifacts.</li> <li>• bones having too little contrast.</li> <li>• skin lines too strong and a Halo around the skin line.</li> </ul> <p>In case configuring P-values is not possible: see "Advanced Settings" .</p>
Transfer syntax	<ul style="list-style-type: none"> <li>• STANDARD: Standard uncompressed encoding</li> <li>• JPEG_LLNH1: JPEG Lossless, Non-Hierarchical (DICOM value= 1.2.840.10008.1.2.4.57) See also further.</li> <li>• JPEG_LNNHF: (in fact, should be 'JPEG_LLNHF' instead):</li> </ul>

	<p>JPEG Lossless, Non-Hierarchical, First-Order Prediction: (Process 14, [Selection Value 1])</p> <p>(DICOM value = 1.2.840.10008.1.2.4.70) and is the default for JPEG lossless.</p> <p>'non-hierarchical encoding' is a JPEG operation mode that does not allow a progressive coding, because hierarchical encoding works with multiple frames, while non-hierarchical encoding doesn't. It is not to be confused with JPEG2000.</p> <ul style="list-style-type: none"> <li>• JPEG_LOSSY:</li> </ul>
Photometric interpretation	Monochrome 2 can for example be applied to fix inverted polarity bug when printing from Impax pre 5.2.2 SU1
Accepts Musica MCE Calcification Enhancement Images	When enabled: MCE processed copies of mammography images are sent to this archive.

## Advanced Settings

### Grayscale correction

Selection of the grayscale correction LUT to be applied. It can be used to correct common system grayscale configuration errors.

- only selectable when the output type is a OD type and the Musica 2 or Musica 3 license is enabled.
- when the output types changes to p-values then this item will change to “no correction”.



*Note: The advanced settings only become editable from model Generic 1.3.0.0 or Standard 1.2.0.0.*

Upload a new version of the model if needed (from the folder C:\agfa\healthcare\nx\bin\DICOMArchiveDeviceModels)

No correction	No correction
Predefined	Correction 1: Grey = 40

E.g. To correct situation where IMPAX monitor set on "NEMA", NX monitor calibrated for gamma 2.20

Correction 2: Grey = 60

E.g. To correct situation where IMPAX monitor set on "Gamma 2.20", NX monitor calibrated for P-Values

Custom

More customized grayscale corrections can be applied here.

The custom setting allows to set a value for black, grey and White.

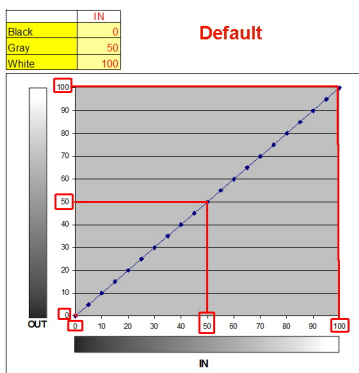


Figure 36: Default 0 - 50 - 100 = no correction

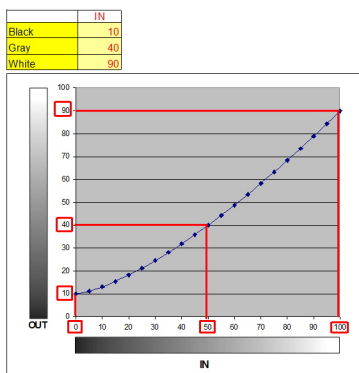



Figure 37: Customized

### Resolution

Resolution

Resolution of the image when sent to archive.

	<p>The Image will be scaled to the number of pixels defined.</p> <p>This setting is not available if GSPS is enabled.</p> <p>This setting is only available for ‘GENERIC’ archive model version 1.3.0.0 and higher! Upload a new version of the model if needed (from the folder C:\agfa\healthcare\nx\bin\DICOMArchiveDeviceModels)</p> <div style="display: flex; align-items: center;">  <p><i>Note: Diagnostic image quality may be lost if the resolution configuration causes downscaling of the image.</i></p> </div>
--	---

<p>Same SOP UID for Presentation and for Processing images</p>	<p>According to DICOM, the SOP instance UID of the raw (“for processing”) image and the processed (“for presentation”) image must be different.</p> <p>However in some situations where the raw image is also sent to a CAD station, the PACS has problems linking the report coming from the CAD station to the original image. Therefore, enabling this setting might help the PACs to link the CAD report to the correct image.</p>
--	--

## Storage Commit

With storage commit, the archive reports back to NX when the archive job is successfully archived.

Setup Storage commit here. Also configure Storage commit in plus in General Configuration.

Time out	Time out on storage commit
Storage commit	Enable or disable storage commit
Enable SSL	Enable secure DICOM for the storage commit communication, requires SSL Certificates!
Hostname IP address IP Stack	Fill in either hostname and IP Stack or IP address (IP Stack detected automatically).
AE title	The AE title to which the storage commit request message is sent
DICOM port	DICOM port to which the storage commit request message is sent

### Related Links

[Workstation Storage Commit](#) on page 43

## Configuring Digitizers

---

### Topics:

- [Introduction](#)
- [Configuring Digitizers System Wide](#)
- [Digitizer Settings](#)

## Introduction

Two types of Digitizers exist: DICOM and Twain Digitizers. The difference is based on the way how they connect to NX.

### Topics:

- [DICOM Digitizers](#)
- [Twain Digitizers](#)
- [Connecting Multiple Digitizers](#)
- [Consequences of Digitizer Selection](#)
- [LGM versus Exposure Index Systems](#)

## DICOM Digitizers

DICOM Digitizers are connected via the network and use the DICOM protocol to communicate with NX. Examples of DICOM Digitizers are SOLO, COMPACT, COMPACT PLUS, CR-25, CR-75, CR 85-X, CR 35-X, ...

## Twain Digitizers

Twain Digitizers are connected via a single firewire interface to the NX. Examples of Twain Digitizers are DX-S and CR30.

## Connecting Multiple Digitizers

In NX, it is not possible to connect (and configure) Digitizers of a different type.

Several DICOM Digitizers can be connected together.

Only one Twain Digitizer can be connected.

Following table gives an overview of possible combinations:

Combining digitizers on one NX	DICOM Digitizer	CR30	DX-S	DX-G
DICOM Digitizer	x	-	-	-
CR30	-	-	-	-
DX-S	-	-	-	-
DX-G (Twain)	-	-	-	-

## Consequences of Digitizer Selection

The configuration of a Digitizer might have consequences on the behavior of the rest of the NX Service and Configuration Tool (and NX).

In case of configuration of CR1B Digitizers (CR75/25...), following features are not available or will give verification errors during activation:




- No "MammoT2" packages selectable (other special mammo packages are selectable though (Magnification spot, ...)).
- Taste settings will have value 0.
- No Musica Micro Calcification Enhancement (MCE) available.

The interactive Musica dialog box in NX will always be unavailable to the regular user for Mammo images (but available for service user).

## **LGM versus Exposure Index Systems**

Refer to the User Manual for more information on LGM versus Exposure Index Systems.

## Configuring Digitizers System Wide
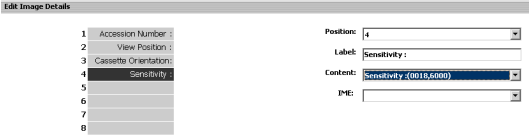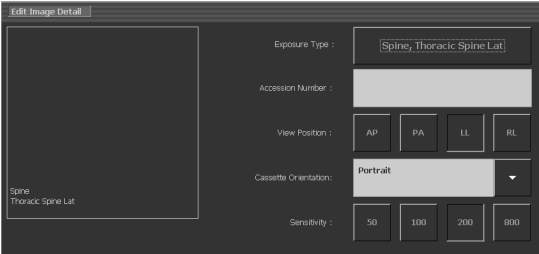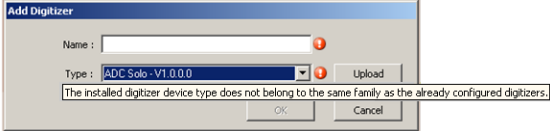
<p>Allowed speed class</p>	<p>You can select up to 4 speed classes (= scanning sensitivity). These speed classes can then be selected by the operator in the Edit Exposure pane of NX (when its visibility is configured in UI Configuration: add 'Sensitivity' attribute).</p>  <p><b>Figure 38: NX Service and Configuration Tool - Allowed Speed Class</b></p>  <p><b>Figure 39: NX - Sensitivity Selection</b></p>
<p>New button</p>	<p>To create\add a Digitizer device.</p> <p>Depending on the already configured Digitizer, a warning symbol is shown next to the Type field. When hovering over it, a clear message is given why a certain selection is not possible.</p>  <p><b>Figure 40: NX Service and Configuration Tool - Add Digitizer dialog box</b></p>
<p>Upgrade Model button</p>	<p>To upgrade existing Digitizer settings</p>

When for an existing digitizer the 'Upgr. Model' button becomes enabled this means that a new version of the model is available in "c:\agfa\healthcare\NX\bin".



**Figure 41: NX Service and Configuration Tool - Upgr. Model button available**

Clicking the 'Upgr. Model' button will load the new version of the model in the NX database and upgrade the current Digitizer to these settings.

## Related Links

[Connecting Multiple Digitizers](#) on page 73

## Configuring the CR Image Recovery Exposure Type

Define the settings to apply when a CR image is received that cannot be linked to a listed exposure. An Age group, examination group and Exposure type will have to be defined.

To configure the CR image recovery exposure type

1. Go to the Recovery Procedure pane in the Digitizer Device Configuration screen.

 A screenshot of a configuration window titled 'Recovery Exposure types'. The window is divided into two columns. The left column is labeled 'Genrad:' and contains three dropdown menus for 'Age Group', 'Exam Group', and 'Exposure Type', each with a downward arrow. Below these is a 'Clear' button. The right column is labeled 'Mammo:' and also contains three dropdown menus for 'Age Group', 'Exam Group', and 'Exposure Type', each with a downward arrow. Below these is another 'Clear' button. The background is white with a thin border.

**Figure 42: Recovery Exposure types**

2. Define an Age group, examination group and Exposure type for Genrad and for Mammo images.

## Digitizer Settings

### Topics:

- [Digitizer Settings General](#)
- [Digitizer Device Settings](#)
- [Emergency Procedure](#)

### Digitizer Settings General

Name	Nickname for this Digitizer
Type	The type
Enable Fast ID (or direct ID)	<p>Fast ID must be enabled when no ID tablet is used. Identification happens then on the Digitizer.</p> <p>Fast ID is mandatory for DX-S, CR 10-X, CR 12-X and CR 30-X(m).</p> <p>Fast ID is optional for CR 25 and CR 35.</p> <p>Fast ID is not possible for CR 75 and CR 85 (as these are buffered Digitizers).</p> <p>Fast ID also needs to be configured in General Configuration – Workstation settings.</p>
Enable Auto Cropping	Turns on or off automatic cropping of the non-relevant image area. Only available for CR 10/12-X.
Genrad Scan Resolution	<p>Default value for the scan resolution of all images except FLFS. Only available for CR 12-X.</p> <p>The user can select another scan resolution before identifying the cassette if the scan resolution attribute is configured. The default value will be marked with “*” in the scan resolution field.</p>
FLFS Scan Resolution	Default value for the scan resolution of FLFS images. Only available for CR 12-X.

### Related Links

[Workstation Fast ID](#) on page 42

[Edit Image Details](#) on page 234

### Digitizer Device Settings

Only for DICOM Digitizers.

Hostname	Fill in either hostname and IP Stack or IP address (IP Stack detected automatically).
IP address	
IP Stack	
AE title	DICOM AE title

### CPF Generation

Only for DICOM Digitizers.

NX must be configured on the DICOM Digitizer. The Digitizer is configured via a cpf-file. It is possible to append the NX parameters to the Digitizer's CPF file. This way it is no longer needed to use the CCM tool.

Default router	Default router on the network, this setting will be written in the CPF file
Subnet mask	Subnet mask of the network, this setting will be written in the CPF file
Modify CPF button	Will load the Digitizer's CPF file and append local NX parameters to it. Uploads the cpf file back to the Digitizer. After this, it is still required to activate the new cpf file on the Digitizer through the standard service procedure.
Create CPF button	Will create a new cpf file for the Digitizer with local NX parameters filled-in. Uploads the cpf file back to the Digitizer.  After this, it is still required to activate the new cpf file on the Digitizer through the standard service procedure.

Following parameters are collected from the NX configuration to be set in the cpf file:

NX setting	To be configured in
ID station name	General Configuration – Workstation settings.
Processing station name	General Configuration – Workstation settings.
Hostname of NX	Digitizer device settings.
Performed station AE title	General Configuration – Workstation settings.
Port	General Configuration – Workstation settings.

Default router	Digitizer device settings.
Subnet mask	Digitizer device settings.
Fast Preview AE title	General Configuration – Workstation settings.
Fast ID AE title	General Configuration – Workstation settings.

### Related Links

[Workstation General Settings](#) on page 40

[Digitizer Settings](#) on page 77

### Emergency Procedure



*Note: Assigning a wrong examination settings in case of an emergency patient may lead to insufficient image quality.*

Define the settings to apply when emergency images are received (e.g. as result of pressing an emergency button on the Digitizer).

An Age group, examination group and Exposure type will have to be defined for each Emergency button.

Exam group	Just a reference to the emergency button on the Digitizer, this field must not be edited.
Exam	Just a reference to the emergency button on the Digitizer, this field must not be edited.
Age group	Configure the age group.
Exam group	Configure the exam group.
Exposure type	Configure the exposure type.

### Configuring Export Destinations



*Note: If no automatic archiving, printing or exporting is configured, unrecoverable image loss can happen if an exam is closed before the images are archived, printed or exported, because it may be automatically deleted by the automatic clean up.*

#### Topics:


- [Configuring System Wide Export Destination Settings](#)

- *Modifying the Properties of DICOM Export Destinations*

## Configuring System Wide Export Destination Settings

In this page, you can configure the **Export Images** functionalities.

In NX, **Export Images** can be found in the Main Menu window:

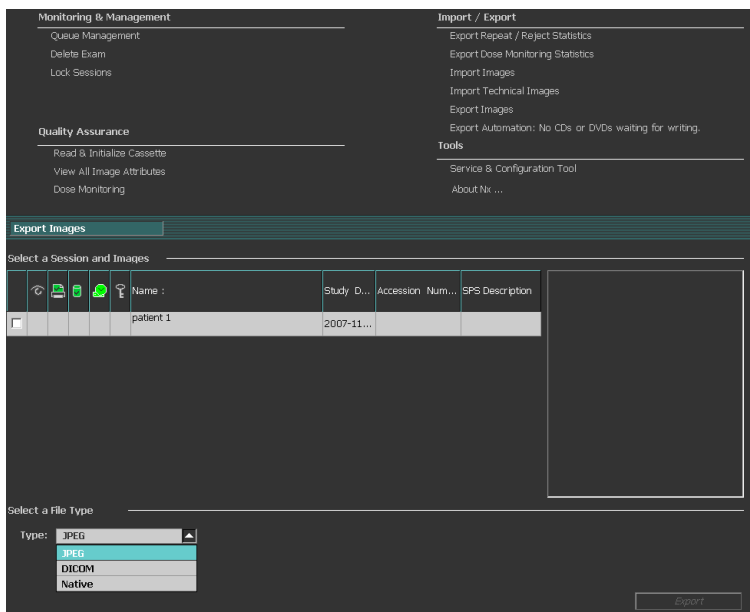

**Figure 43: NX - Export Destinations**

Three types of exports exist:

- DICOM Export
- JPEG Export
- Native Export



*Note: 'Export to native NX format' is only available for service (when logged in with an account that has service rights).*

### Topics:

- [DICOM Export](#)
- [JPEG Export](#)
- [Native Export](#)

### DICOM Export

DICOM export in NX is only possible to CD\DVD.



It is not possible to import the DICOM images again in NX.


The images can be viewed with any DICOM-compliant viewer. Optionally a Viewer can be written on the disk with the exported image data. This can be established with the **Include DICOM viewer** checkbox.

The CD/DVD can serve as a “referral CD/DVD”, an electronic version of the patient handout. The private practitioner might also want to use this as a personal archive.

It is possible to select one or more images from an exam or several exams to export. A rejected image can also be exported.

Since the DICOM export is standardized, it is NX version independent.
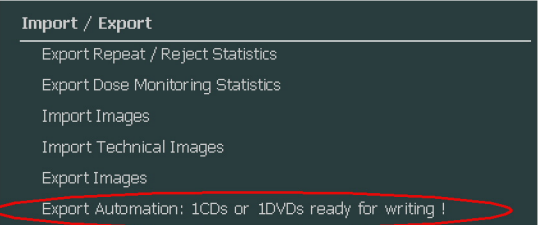
<p>Enable export automation</p>	<p>When enabled, all images of all exams will be automated for DICOM export after closing. All data is copied in an export automation buffer.</p> <p>Export to CD/DVD can be started by clicking following link in the Main Menu window of NX:</p>  <p><b>Figure 44: NX Main Menu - Import/Export section</b></p> <p>the nx automatic cleanup process (which runs every hour) does not remove exams that are waiting to be exported in the export automation buffer. only after this buffer is emptied, by burning cd/dvds, the exams will be marked for cleanup again.</p> <p>in the worklist, an automation icon is shown.</p> <div style="display: flex; align-items: center;">  <p><b>CAUTION:</b> if the export automation buffer is full, no new exams will be added. they may be deleted by the automatic clean up after some time. this can cause unrecoverable image loss. Empty the buffer in time, by performing the export to cd/dvd. export the exams manually, that were not exported automatically after the buffer ran full.</p> </div>
<p>sopclass</p>	<p>select the proper sop class for exporting. it is possible to select more than one sop class.</p>

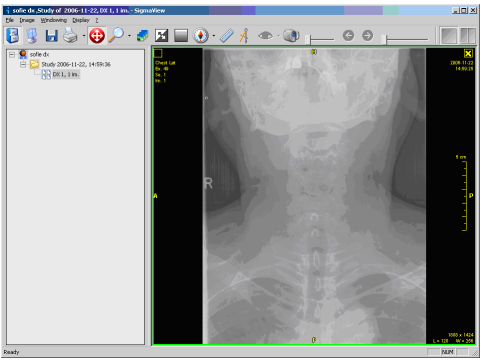include dicom viewer	<p>when enabled, the sigmaview dicom viewer will be written to the cd\dvd together with the exported images.</p>  <p><b>Figure 45: dicom viewer</b></p>
Include patient demographics	<p>When disabled, the export will be anonymous. If export automation is enabled, this option is not available and patient demographics are always included in the exported image.</p>
GSPS supported	<p>When enabled: the GSPS will be exported together with the image.</p>
Output type	<p>Output type to be used when exporting.</p> <p>Possible output types are dependent of the selected SOP class.</p>
Buffer size	<p>Defines the size of the export automation buffer. I.e. the size of the buffer that is available for storing images before they are burned on CD/DVD.</p>



*Note: The DICOM export is IHE compliant only if the user or the RIS has provided a value for the Patient ID field.*

## Related Links

[Storage](#) on page 56

## JPEG Export

JPEG export in NX is possible to a folder only.

To be used for e.g. didactical purposes in a slide show or a scientific paper. JPEG images are certainly not to be used for diagnostic purposes.

It is not possible to import the JPEG images again in NX.

It is possible to select one or more images from an exam to export. A rejected image can also be exported.

There is no viewer exported together with the images (as for DICOM export).

Used compression scheme: Lossy encoded, as is used in Transfer syntax: JPEG Baseline, Lossy encoded (UID 1.2.840.10008.1.2.4.50).

Include patient info in filename	<p>When enabled: the filename contains the patient name and patient ID.</p> <p>When disabled: the export is anonymous.</p>
----------------------------------	--

## Native Export

This functionality is provided for service only.

Native export in NX is possible to a local folder or CD\DVD.

The exported images can be imported back to NX, with the following constraints:

- NX-specific exam semantics are lost. An imported exam structure is created when the images are imported, with defaults for missing exam information. Some functionality will be disabled for imported exams.
- The used exposure type name will be shown, but the original exam tree is not exported along with it.
- There is no guarantee that images can be imported back on a different version of NX.
- Archive, print automation and MPPS at 'close exam' is completely disabled on these imported exams. Closing an imported exam has no further consequences.
- The clean up date of the exam is set to the time of import. This way, it will be treated in a similar way as a newly created exam by the clean up mechanism.

It is possible to select one or more images from an exam to export. A rejected image can also be exported.

There is no viewer exported together with the images (as for DICOM export).

Include patient demographics	<p>When enabled: the export contains the patient demographics data.</p> <p>When disabled: the export is anonymous.</p>
------------------------------	--


## Modifying the Properties of DICOM Export Destinations

### Topics:


- [General](#)
- [DICOM Export Overview](#)
- [Exporting via CMS](#)
- [Viewing DICOM Export](#)

### General


The list of created DICOM export destinations is listed in the NX Main Menu window:

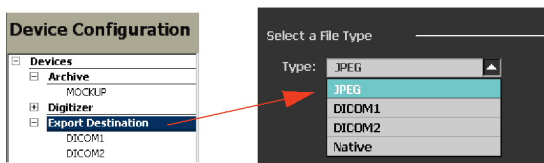

**Figure 46: DICOM Export Destinations**

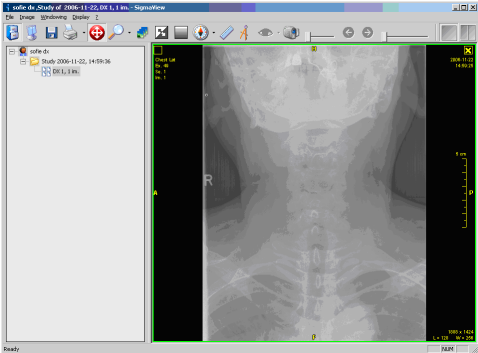name	nickname for this export destination. will be shown in nx (see above).
sopclass	select the proper sop class for exporting. it is possible to select more than one sop class.
include dicom viewer	<p>when enabled, the sigmaview dicom viewer will be written to the cd\dvd together with the exported images.</p>  <p>The screenshot shows a window titled '1. wife de Study of 2006-11-02, 00 L 1 im - Sigmaview'. It features a toolbar at the top, a file explorer on the left showing a folder 'Info-01' with files '01 Study-2006-11-02_14:59:36' and '05 L 1 im', and a large central area displaying a grayscale chest X-ray. The X-ray is labeled with 'R' for right and 'L' for left. The status bar at the bottom indicates 'Ready' and 'Page 1 of 1'.</p>

**Figure 47: dicom viewer**

Include patient demographics	<p>Default setting for the "Include Patient Demographics" checkbox in the NX export pane.</p> <p>So in NX it will still be possible to enable or disable this:</p>  <p><b>Figure 48: NX - Include Patient Demographics check box</b></p> <p>When disabled, the export will be anonymous.</p>
GSPS supported	When enabled : the GSPS will be exported together with the image
Output type	<p>Output type to be used when exporting</p> <p>Possible output types are dependent of the selected SOP class.</p>

## DICOM Export Overview

Overview of the DICOM Export SOPClasses.

	DICOM Export for presentation	DICOM Export for processing
<b>SOPClass</b>	<b>[CR for presentation]</b> <b>[DX for presentation]</b> <b>[MG for presentation]</b>	<b>[DX for processing]</b> <b>[MG for processing]</b>
Image (RAW) + Musica processing + W/L + collimation	Processed pixels + LUTs	RAW pixels only
Annotations	GSPS or Burned In	Ignored
Measurements		
Shutters		
Zoom	GSPS or ignored	
Markers	Always burned in	

	DICOM Export for presentation	DICOM Export for processing
SOPClass	[CR for presentation] [DX for presentation] [MG for presentation]	[DX for processing] [MG for processing]
Exam related data	Ignored	
Bitmap shutter (for background darkening)	GSPS or ignored	Ignored

## Exporting via CMS

When exporting on CMS, the export configuration of the CMS itself will be used! The CMS pushes its configuration to the in-room NX.

The actual export to CD/DVD or folder (for JPEG) happens on the CMS itself.

It is also possible to select exams of different NX workstations on CMS.

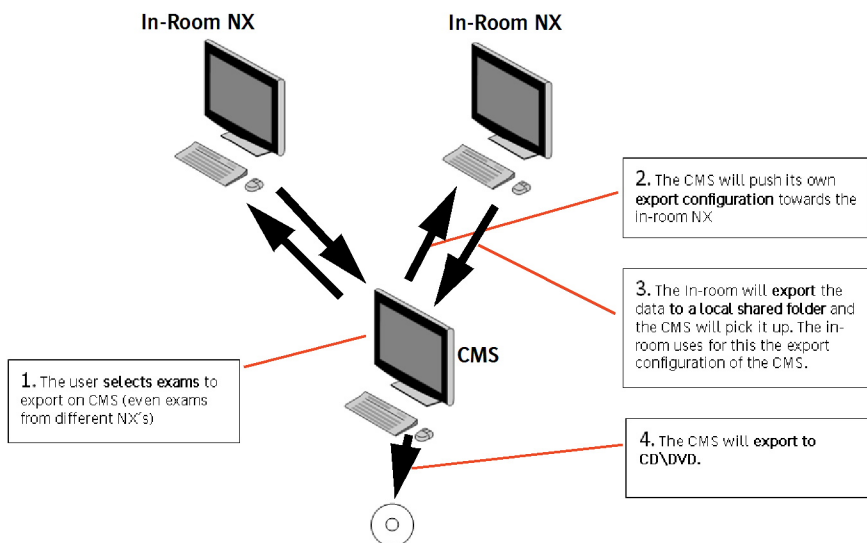


Figure 49: Exporting via CMS - Overview

## Viewing DICOM Export

The DICOM Export CD/DVD contains software to view the exported images. Minimum PC requirements to use the viewing software are:

- CPU: 1GHz Pentium-4
- RAM: 512 Mb
- Display: resolution of 1024 by 768 pixels (32 bits)
- Operating System: Windows Vista Business (32 bit) SP2, Windows 7 Business (32 bit) SP1, Windows 8, Windows 8.1

## Configuring ID Tablet

---

### Topics:

- *Configuring ID Tablet System Wide*
- *Configuring Properties of ID Tablet*

## Configuring ID Tablet System Wide

Only one ID tablet can be created.

Only one ID tablet model (type) is available.



*Note: 'Automatic cassette identification' needs to be configured in General Configuration – configure workstation settings:*

**Workstation settings**

---

General Settings \_\_\_\_\_

ID station name: **VAM1850**

Performed Location: \_\_\_\_\_

Processing station name: **VAM1850**

Character Set:  Arabic (ISO IR 127)  
 Chinese - Simplified (GB18030)  
 Chinese - Simplified (ISO 2022 GBK)  
 Chinese - Traditional (ISO 2022 B5)

Enable automatic cassette identification

**Figure 50: NX Service and Configuration Tool - Workstation Settings**

With **Automatic cassette identification**, the identification is automatically started on insertion of the cassette in the ID tablet. The settings of the exposure, which is selected at that moment in NX, are used.

## **Configuring Properties of ID Tablet**


Only one ID Tablet can be configured.

## Configuring Monitors

**Figure 51: NX Service and Configuration Tool - Configuring Monitors**

Setup the attached monitor. Some pre-defined monitor types exist. A type also contains the screen resolution in horizontal and vertical number of pixels. During startup of NX, the resolution of the configured type is compared to the actual value in Windows. If there is a mismatch, a message will be displayed and you'll need to correct it.

Further, the type also contains pixel spacing values for optimal font display on higher resolution monitors.

Name	Nickname for this monitor
Description	Description
Type	The configured type
Gamma	Gamma setup
Test image	Select a test image. This image will be shown when clicking the View button.
Modify button	<p>Allows to change the type</p>  <p><b>Figure 52: NX Service and Configuration Tool - Modify Monitor dialog box.</b></p> <p>More pre-defined types can be uploaded via the Upload button.</p>
View button	Shows the selected test image on the screen

## Configuring Printers

---



*Note: If no automatic archiving, printing or exporting is configured, unrecoverable image loss can happen if an exam is closed before the images are archived, printed or exported, because it may be automatically deleted by the automatic clean up.*

### Topics:


- *Configuring System Wide Printing*
- *Modifying the Properties of Existing Printers (Changing Printer Profiles)*


## Configuring System Wide Printing

### Topics:

- [Printing Main Settings](#)
- [Printer Models](#)
- [Upgrade Existing Printer Settings](#)
- [Print Sheet and Layout](#)
- [Sheet Text Box & Image Text Box](#)
- [Configuring Bitmap Files Offline](#)

### Printing Main Settings

<p>Enable printer automation</p>	<p>If enabled, all images of an exam will be submitted for DICOM print after the Close And Send button in NX is pressed.</p> <p>Printer automation can be disabled for specific exposures.</p>
<p>Default printer profile</p>	<p>Printer to be used in NX when a new print sheet is made:</p>  <p>The screenshot shows a vertical menu titled 'Print' with several icons and dropdown menus. Red arrows point from text labels to specific icons: 'Deletes current print sheet' points to a trash can icon, 'Makes new print sheet' points to a printer icon with a plus sign, and 'Filmsize and printer used for this sheet' points to a dropdown menu showing '11INx14IN firc'. At the bottom of the menu, there are navigation arrows and the text '1 / 3'.</p> <p><b>Figure 53: NX - Printer Profile Selection</b></p>
<p>Default film size</p>	<p>Film size of default printer to be used in NX when a new print sheet is made (see above)</p>
<p>New button</p>	<p>To create a new printer on NX, enter a nickname and select a type.</p>

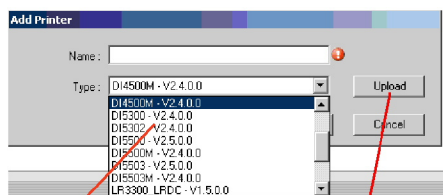

Printer models currently available in the NX database. Their version number is shown.

By using the UPLOAD button, new models can be loaded into the NX database or older models can be updated.

**Figure 54: NX Service and Configuration Tool - Add Printer dialog box**

The version number (e.g. V2.5.00) is just the version number of the type itself.

Delete all button	Removes all configured printers.
Restore button	Re-sets the image and sheet text box settings back to factory values.

## Related Links

[Automation](#) on page 172

## Printer Models

Printers are configured in NX Service and Configuration Tool starting from printer models.

A printer model contains predefined settings as:

- supported film sizes\types
- Dmin\Dmax
- Interpolation settings
- ...

These printer models are available on NX in two places:

- the NX database
- as xml files in c:\agfa\healthcare\NX\bin\DICOMPrinterModels folder

More than 60 different xml files are released. Each xml file lists the settings of one model.

Each model has a version number.



Existing printer profiles are not modified with an upload. You can always use the 'Upgr. Model' button

An upload cannot be undone.


Of course, it is always possible to change the printer settings in the profile

Xml Printer model files can be used on all versions of NX and are available to the service organization.

## Upgrade Existing Printer Settings

When for an existing printer the 'Upgr. Model' button becomes enabled; this means that a new version of the model is available in: c:\agfa\healthcare\NX\bin\DICOMPrinterModels.

Clicking it will load the new version of the model in the NX database and upgrade current printer to these settings.

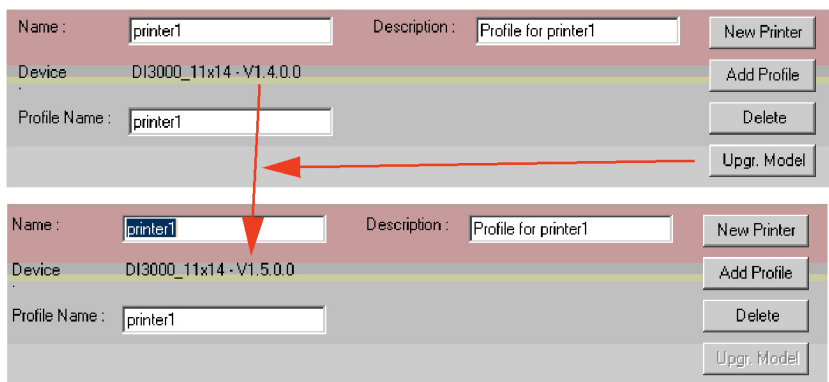


**Figure 59: NX Service and Configuration Tool - Upgrade Printer settings**

## Print Sheet and Layout

This area provides the easiest way to configure printing on the system, you simply link a cassette size to a film size and a configured printer. Any exceptions to this general rule can be configured in examination Tree Configuration > Printer Configuration.

<p>Cassette &amp; film size</p>	<p>Link a cassette to a film size.</p> <p>When you also link a film size to a printer profile (see further), automatic printing becomes possible when a cassette of a certain size is identified.</p> <p>These settings are only used for exposure types of which the FilmSize setting is set to DEFAULT:</p>
---------------------------------	---

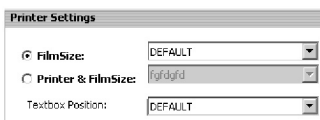

**Figure 60: NX Service and Configuration Tool - Printer Settings - Cassette and Film Size**

For exposure groups this setting is not used.




*Note: 'Sheet size' is the same as 'film size'.*

Film & profile size

Link a film size to a printer.


These settings are also used for all exposure types for which the FilmSize is set to a specific value:

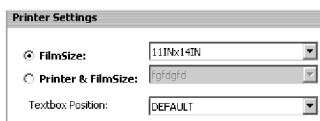

**Figure 61: NX Service and Configuration Tool - Printer Settings - Film and Profile Size**

For exposure groups:

This setting is also used to determine the printer for exposure groups that have no specific printer defined (but DEFAULT).



**Figure 62: NX Service and Configuration Tool - Printer Settings - Print Sheets**

## Related Links


[Printer Settings](#) on page 173

## Sheet Text Box & Image Text Box


Possibility to configure the text box of the complete print sheet (=sheet text box) and the text box of a single image (=image text box).

A text box is composed out of different cells and rows.

The attributes that can be configured for an image text box are a sub-set of the attributes that can be configured for a sheet text box. Therefore, notice the difference of the text cell editor:

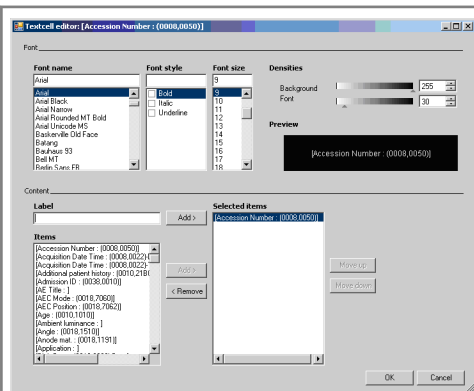

**Figure 63: NX Service and Configuration Tool - Text Cell Editor for the Sheet Text box.**

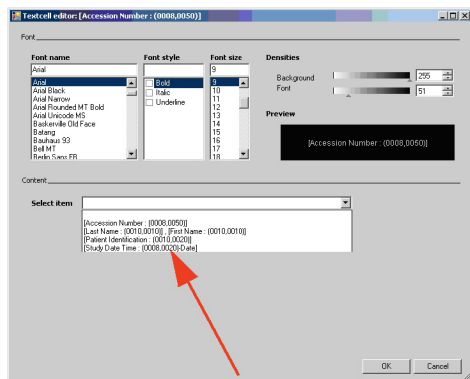

For an image text box, only attributes that are configured on sheet text box level can be selected.

**Figure 64: NX Service and Configuration Tool - Text Cell Editor for the Image Text box.**

At run-time, NX applies some logic on the rendering of these textboxes. This means that some attributes may not be shown even when configured. The rules are:

- a 1/1 layout only has a sheet text box never an image box
- on other than 1/1 layouts you can have both, but
- an image text box is only shown when it contains image related attributes (e.g. acquisition date \ time), otherwise the image text box is not shown.

- if both sheet and image text box are to be shown, then sheet text box attributes that are already in the image text box are not shown.

Further:

Sheet text boxes on a 1/1 layout are shown in the image for true size and outside the image for best fit.



*Note: Sheet textbox positioning can be overruled per exposure type in the exam tree set-up (but only for 1/1 layouts).*

All these settings can be tested (printed out) from within the NX Service and Configuration Tool by using the ‘Test profile’ button in the printer set-up screen!


Reset the sheet and image text box settings by using the ‘Restore...’ button.

### Cell Types


When clicking on a cell, the cell type is indicated in:



**Figure 65: NX Service and Configuration Tool - Cell Types**
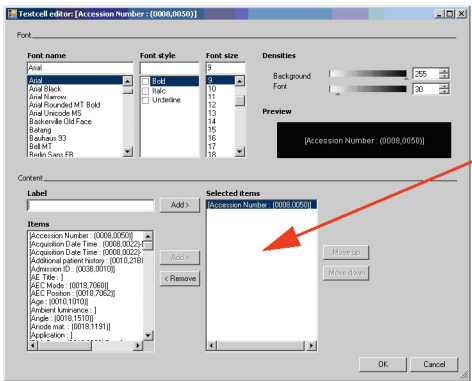
<p>Text</p>	<p>Possibility to add:</p> <ul style="list-style-type: none"> <li>• plain text (fill in Label field)</li> <li>• attributes (which will be resolved at run time: their actual value will be filled in)</li> </ul> 
<p>Scale</p>	<p>True size indicator (or % scaled)</p>

**Figure 66: NX Service and Configuration Tool - Cell Types - Content of the cell**

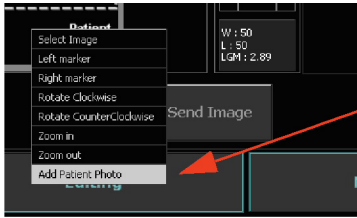Dose bar	Graphical representation of the dose value (LGM or EI) relative to the dose reference value for this exposure.
Bitmap	<p>Only possible on a sheet text box.</p> <p>Select a fixed bitmap or PATIENT_PHOTO.BMP.</p> <p>Selecting PATIENT_PHOTO.BMP allows you on NX to add a patient photo:</p>  <p><b>Figure 67: NX - Patient Photo selection</b></p> <p>When selecting a bitmap in an offline NX Service and Configuration Tool make sure to copy the bitmap file also to the online NX.</p>

## Configuring Bitmap Files Offline

When configuring bitmaps to be printed on film in an offline NX Service and Configuration Tool, you should also manually copy over the bitmap file to the online NX system, in the following directory:

C:\Agfa\Healthcare\NX\Configuration\BitmapFiles (or you can always do the copying again through on the online system).

On an offline NX Service and Configuration Tool system the bitmap file is copied to C:\Agfa\Healthcare\NX\Offline.Config.Tool.x.x.xxxx\Bin\DataFiles\Configuration\BitmapFiles

While on an online system this directory is:

C:\Agfa\Healthcare\NX\Configuration\BitmapFiles

## Modifying the Properties of Existing Printers (Changing Printer Profiles)

### Topics:

- [Main Settings](#)
- [Device Settings](#)
- [Image Sheet Settings](#)
- [Advanced Settings](#)
- [Medium Settings](#)

## Main Settings

Name	Name of the physical printer, only used in the NX Service and Configuration Tool. Used for all profiles for this printer. Changing it, will change it for all profiles for this printer.
Device	The model and version.
Profile name	Enter a nickname for this printer profile. This name will be used in NX.
Description	Description.
New printer	Makes a new printer (profile). Profile name = printer name.
Add profile	Makes a new profile for this physical printer. So makes a copy of current printer settings in a new printer profile.
Delete	Deletes current printer profile
'Upgrade Model' button	When this button becomes enabled, a new version of the model is available in  c:\agfa\healthcare\NX\bin\DICOMPrinterModels.  Clicking it will load the new version of the model in the NX database and upgrade current printer profile to these settings.

## Related Links

[Printer Models](#) on page 94

## Device Settings

Hostname IP address IP Stack	Fill in either hostname and IP Stack or IP address (IP Stack detected automatically).
DICOM port	The network port the printer SCP is listening on.
Enable SSL	Secure printing, requires SSL set-up (certificates) on both sides.
Priority	The priority of the DICOM print jobs sent to this printer


Use N-Events	<p>When enabled, NX waits for N-Events from the printer reporting back to NX the status of print jobs.</p> <p>A print job will be marked as DONE only when the print sheet is available in the output bin.</p> <p>When disabled, NX considers a job printed when it left the print queue of NX and is spooled by the printer.</p> <p>When ‘film session printing’ is enabled, the N-events will represent the status of the whole FS (with possible multiple sheets). Otherwise, the N-Events represent the status of 1 print sheet.</p>
AE-title	The DICOM AE-title of the printer’s SCP.
Film sizes	Lists the available film sizes as defined in the model, possible to uncheck some. The film size is shown in the list as soon as it is supported by a medium type.
Test connection	<p>Ping, checks the IP address.</p> <p>Followed by a DICOM ping (Verification SOP class), which checks the AE-title and port.</p>

## Image Sheet Settings

Background density	The density of the area not occupied by the image in the image cell.
Border density	The density of the border of the print sheet and of empty image cells.
Ruler	Whether or not a ruler should be printed on film.
View box illumination	<p>For Musica: leave this value at default</p> <p>For Musica 2 or Musica 3: Enter the luminance of the light box in <math>\text{cd}/\text{m}^2</math>. It has to be measured with a light meter. You can also set the value of 2000.</p> <p>See also Pixel format in “Advanced Settings”</p>
Reflected ambient light	<p>For Musica: leave this value at default.</p> <p>For Musica 2 or Musica 3: Enter the diffuse reflection luminance of the viewing area in <math>\text{cd}/\text{m}^2</math>, measured with a light meter. You can also set the value of 1.</p>

Test profile	Allows to print a test sheet from the NX Service and Configuration Tool.
--------------	--

## Advanced Settings

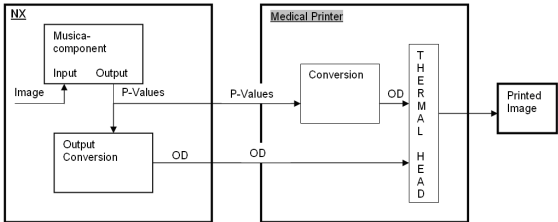Magnification type	<p>Defines the interpolation used when images need to be scaled. This is done on NX and not on the printer as NX makes a complete sheet bitmap for the printer using the complete printable area of the printer. Next to this, NX sends MAGNIFICATION NONE to avoid the printer from interpolating. If the printer doesn't support this, REPLICATE is sent.</p> <p>The preferred value for Musica 2 and Musica 3 is BICUBIC BELL hi res.</p>
Smoothing factor	<p>Smoothing factor belonging to the magnification type.</p> <p>The preferred value for Musica 2 and Musica 3 is 0.9.</p>
Configuration info	<p>Printer Device specific Configuration Info.</p> <p>The preferred value for Musica 2 and Musica 3 is Perception_LUT linear.</p>
Pixel format	<p>Combination of the pixel type (P-values or OD) and the number of bits.</p> <p>The preferred value for Musica 2 and Musica 3 is 12bit pvalue.</p> <p>Background info:</p> <p>Using p-values will achieve a consistent greyscale perception of the images, independent of the viewing media, like diagnostic softcopy monitors, referral workstation monitors, hardcopy film, and this in different light conditions.</p>  <pre> graph LR     subgraph NX         Image[Image] --&gt; Musica[Musica-component]         Musica --&gt; PValues[P-Values]         Musica --&gt; OutputConv[Output Conversion]         OutputConv --&gt; OD1[OD]     end     subgraph MedicalPrinter[Medical Printer]         PValues --&gt; Conversion[Conversion]         Conversion --&gt; ThermalHead[T H E R M A L H E A D]         OD1 --&gt; ThermalHead     end     ThermalHead --&gt; PrintedImage[Printed Image]   </pre> <p><b>Figure 68: NX Service and Configuration Tool - Pixel Format</b></p>

	<p>1. In case an image in P-Value format is transmitted, there will be negotiation for PLUTs.</p> <p>When the SCP supports PLUTs, NX will send 'PLUT Shape', having the value 'IDENTITY'. So, no Look Up Table (PLUT Table) will be sent, only the string 'IDENTITY'.</p> <p>The printer will perform the conversion from P-Values to OD image format.</p> <p>Illumination (2010,015E) and Reflected Ambient Light (2010,0160) are used to recover Optical Density information from P-Values.</p> <p>But since these values (view box settings) have already been optimized/manipulated in Musica, the default values should be used.</p> <p>2. In case of an image in OD format, there will be no negotiation for PLUTs and no PLUT will be sent.</p> <p>The <b>DICOM Configuration Info</b> field, filled in by the user, has to contain the perception LUT to be applied by the printer on the image. The applicable settings depend on the printer-type and are for Agfa printers: linear (default), kanamori, kanamorilike (75.220).</p> <p>The view box settings have no meaning here - no PLUT values are used.</p>
Film session printing	<p>Enabled: NX will send all sheets of an exam in one DICOM film session (FS) to the printer (if they all are to be sent to the same printer), with the print command (N-Action) on FS level. This guarantees that all films of one exam are laid off in the same printer bin.</p> <p>Disabled: NX will send all sheets in different DICOM film sessions (FS) to the printer (one film box (FB) per FS).</p>
Film destination	(2000,0040) 'Bin' allows to specify a bin number further.
Film destination bin no.	BIN no to be used when film destination = BIN.

## Medium Settings

Medium type	Medium type to be used by this printer profile.
-------------	---

Min density	Minimum density for this printer profile. Value between 0 and 4.
Max density	Maximum density for this printer profile. Value between 0 and 4.

## Configuring Priors

---

This section describes what should be configured in the NX station to be able to access the Viewing Priors interface.

The precise configuration depends on the version of IMPAX (or WEB1000) that is installed.

- URL WEB1000 R4.1& R5.x:  
 http://<server>/agfa/QueryForStudies.jhtml?  
 propertiesfile=QueryForStudiesNX&whereclause=  
 Authentication does not require a Domain Name.
- URL IMPAX 6.2:  
 AgfaImpaxBridge://C:\Program Files\Agfa\AgfaImpaxBridge  
 \BridgeRemote.exe/QueryForStudies?configfile=bridge\_settingsNX.xml  
 Authentication requires a Domain Name.
- URL IMPAX Results Viewer:
  - Using https protocol: AgfaImpaxResultsViewer://<server>/  
 ResultsViewer/emr.aspx?
  - Using http protocol: AgfaImpaxResultsViewerNonSecure://  
 <server>/ResultsViewer/emr.aspx?
 Authentication requires a Domain Name.
- URL IMPAX Data Center (Xero):
  - Using https protocol: AgfaXero://<server>/?
  - Using http protocol: AgfaXeroNonSecure://<server>/?
 Authentication does not require a Domain Name.
- URL Impax SE Web Client:
  - Using https protocol: AgfaImpaxSE://C:\Program Files\Agfa  
 HealthCare\SE Web Client\SigmaRemote.exe/<server>
  - Using http protocol: AgfaImpaxSENonSecure://C:\Program Files  
 \Agfa HealthCare\SE Web Client\SigmaRemote.exe/<server>
 Authentication does not require a Domain Name.



*Note: The name of the IP address (<server>), the User name and the password are defined by the IMPAX configuration.*



*Note: The first time Viewing Priors is used, some dialogs will pop up to configure the communication to the WEB1000 (e.g. Java install, certificates,...). These dialogs can be confirmed. This will happen for each different user!*



*Note: If a Domain Name is required, this should be configured as part of the user name, which is then of the format <username>@<domainname>.*

Consult the service documentation of the Prior Viewing providers for further details on:

- Not all filters (Study Date, Study Status, Modality and Body Part) are supported by all Prior Viewing providers.
- Required Security Settings (e.g. Internet Explorer settings, Certificates, ...) may differ depending on the Prior Viewing provider.
- Additional software may need to be installed depending on the Prior Viewing provider.

## Configuring RIS

---

### Topics:

- *Configuring System wide RIS settings*
- *Modifying the Properties of Individual RIS*
- *RIS Mapping*

## Configuring System wide RIS settings

Procedure:

In the Device overview pane, click **RIS**.


The main form for configuring RIS will appear.

### Topics:

- [Adding a New RIS](#)
- [Configuring Main RIS Settings](#)

### Adding a New RIS

With the **New** button, a new RIS device can be created.

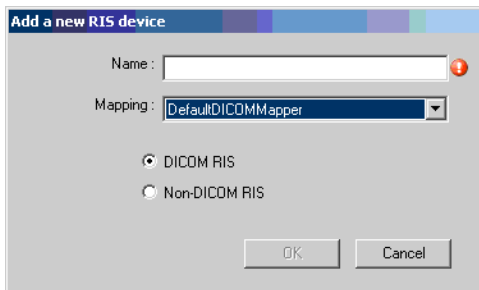

**Figure 69: NX Service and Configuration Tool - Add new RIS device**

Procedure:

1. Click the **New** button.
2. Fill in a nickname for this RIS.
3. Select a pre-defined mapping.
4. Select whether it concerns a DICOM or a non-DICOM RIS.


### Related Links

[RIS Mapping](#) on page 115

### Configuring Main RIS Settings

Initial RIS device	<p>Defines the default RIS device of the system.</p> <p>More than one RIS device may be configured.</p> <p>The 'initial RIS' defines the RIS which will be used on startup of NX.</p>
--------------------	---

At runtime you can switch between different RIS systems in the worklist screen:

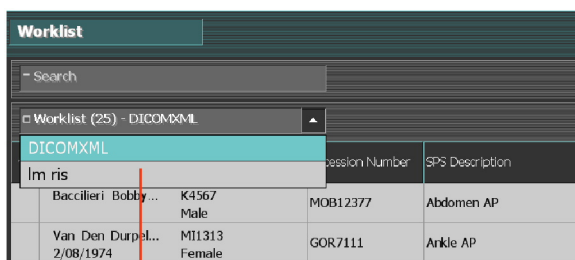

Select the RIS here, a query is automatically done

**Figure 70: NX - Initial RIS Device**

Use Japanese protocol code guideline JJ1017	<p>To be enabled for Japanese protocol codes.</p> <p>I.e. an extra sequence (0040,0440) is used in Scheduled protocol code sequence (0040,0008).</p> <p>Also, for automatic exposure selection, it is not enough to map to 0040,0008 'Protocol code value'. Two extra attributes must be used, separated by slashes, see JJ1017 guidelines.</p>
Use non-DICOM protocol codes	<p>When this function is enabled, protocol codes longer than 16 characters are accepted.</p> <p>When disabled, NX Service and Configuration Tool checks on maximum size of 16 characters.</p> <p>A protocol code longer than 16 characters is never sent to the archive (independent of the setting of this flag).</p> <p>Excel files (used to generate protocol code xml files) also accept more than 16 characters.</p>

### Related Links

[Japanese Protocol Codes](#) on page 125

[Automatic Selection of Exposure, Exam or Exposure group](#) on page 123

## Modifying the Properties of Individual RIS

Procedure:

Select a RIS from the tree view.

### Related Links

*RIS Mapping* on page 115

**Topics:**


- *Main Settings*
- *Connection Type Settings for DICOM RIS*
- *Connection Type Settings for non-DICOM RIS*
- *MPPS Destination Settings*


**Main Settings**

- Name

Nickname for this RIS device

- Query Type (only for DICOM RIS)

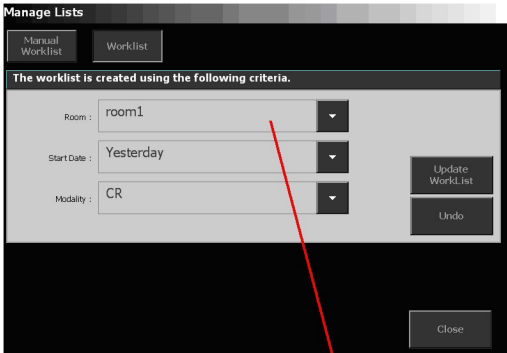
<p>Broad</p>	<p>Default mode.</p> <p>In this mode, the fields SPS Start Date, modality and Default Scheduled Station AE-Title are used in the query to the RIS.</p> <p>It is possible to change them at run time in NX in the Manage Lists window in the Worklist of NX:</p>  <p>The configured 'Scheduled station AE titles'</p> <p><b>Figure 71: NX - Manage Lists</b></p>
<p>accession number</p>	<p>in this mode, the user must enter an accession number in the worklist window of nx which is used in the query:</p>

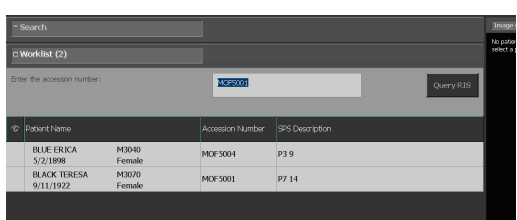

**Figure 72: nx - enter accession number**

In this mode, the fields SPS start date, modality and Default scheduled station AE-Title are NOT used in the query to the RIS.


### Connection Type Settings for DICOM RIS

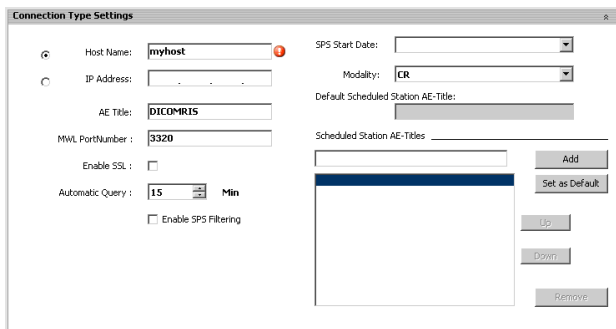

**Figure 73: NX Service and Configuration Tool - Connection Type Settings pane**


Hostname	Fill in either hostname and IP Stack or IP address (IP Stack detected automatically).
IP address	
IP Stack	
AE title	DICOM AE title of the DICOM RIS
MWL port number	Port number of the DICOM RIS
Enable SSL	Enable secure DICOM (SSL Certificates required)
Automatic query	Interval in minutes NX should query RIS 0 means: no automatic query

<p>Enable SPS filtering</p> <p>this filtering only works with a DICOM RIS which sends a value for studyuid, for a non-DICOM RIS no SPS can be filtered away.</p>	<p>When this flag is enabled, NX checks - during receipt of new worklist items from the DICOM RIS after a query - whether a 'started' or 'completed' SPS exists already on NX.</p> <p>If it already exists, then the received SPS is NOT added again to the NX worklist (filtered away). This can help to keep the worklist short if it is not kept up to date on the RIS side.</p> <p>When this flag is disabled (default behavior), the system will not check if the SPS already exists on NX. This could result in adding the same SPS to the worklist more than once.</p> <p>E.g. you could have two entries in the worklist with name 'John Doe', one with an 'eye' icon in front and one without this icon.</p> <p>Checking on SPS equality is done by comparing 6 fields of two SPS' (patientname, sex, birthdate, patientid, spsid, studyuid).</p>
<p>SPS start date</p>	<p>(0040,0002)</p> <p>The default value for the SPS start date in the Modality Worklist (MWL) query. Can be left empty.</p>
<p>Modality</p>	<p>(0008,0060)</p> <p>The default value for the modality type in the MWL query. Can be left empty.</p>
<p>Default scheduled station AE-Title</p>	<p>(0040,0001)</p> <p>The scheduled AE title to be used during the MWL query. Can be left empty.</p>
<p>Scheduled station AE titles</p>	<p>(0040,0001)</p> <p>The list of possible scheduled AE titles. This makes it possible to select stations in the Manage Lists screen in NX.</p>

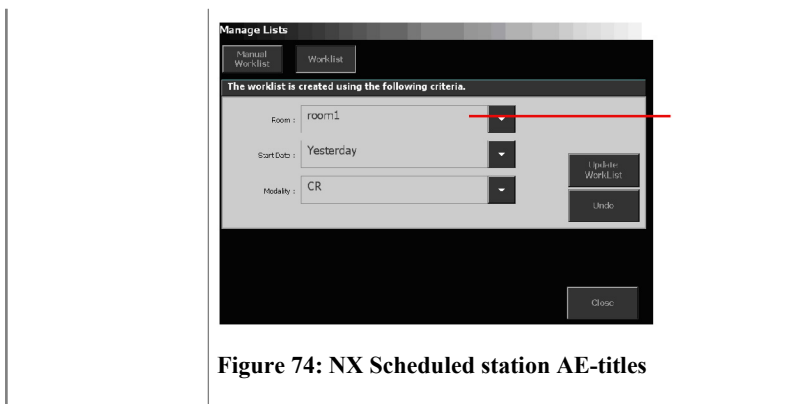

**Figure 74: NX Scheduled station AE-titles**

## Connection Type Settings for non-DICOM RIS

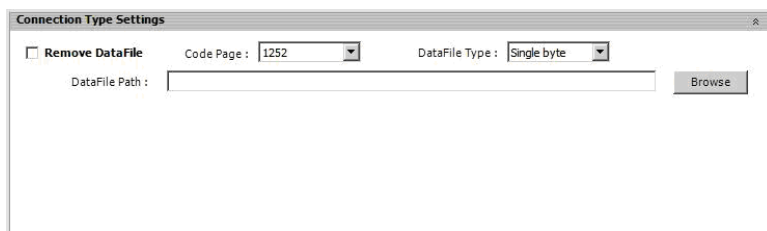

**Figure 75: Connection Type Settings pane (non-DICOM)**

Depending on the RIS type, these settings can be configured:

Remove Datafile	Enable this to remove the data file after each query. It is recommended to enable this option, to make the latest RIS data available in NX.
Code Page	ASCII code page to be used
DataFile Type	Select <b>Single byte</b> for ASCII file or <b>Multi byte</b> for XML file
DataFile Path	File name and path of the data file
Parameter File Path	File used to convert the delimited worklist
Automatic Query	Time interval in minutes between the queries
User Program Path	File name and path of the user program to be executed

## MPPS Destination Settings

Only applicable to DICOM RIS

Send out MPPS	Enabling or disabling sending of MPPS.  If MPPS is enabled, editing of patient data in NX will be prevented independent of the 'Lock patient demographics' settings made in the Workflow management. (In fact, editing is still allowed here until the first image arrives).
Hostname IP address IP Stack	Fill in either hostname and IP Stack or IP address (IP Stack detected automatically).
AE Title	AE title of the MPPS destination
Port number	Port number of the MPPS destination
Enable SSL	Enable secure DICOM
Modality	CR, DX, MG or RF  Value to be used in the MPPS

## RIS Mapping



### WARNING:

Information from the RIS can be lost because of wrong mapping of incoming SPS attributes to the internal NX data structure.

The purpose of RIS mapping in NX is:

- Filling-in of patient and exam data from RIS in the correct NX data structures (= obtained through mapping)
- Automatic exposure (or exam or exposure group) selection in NX starting from protocol codes coming from the RIS

RIS mapping is required for DICOM and non-DICOM RIS.

### Related Links

[Automatic Selection of Exposure, Exam or Exposure group](#) on page 123

### Topics:


- [Basic Mapping](#)
- [More Details on Mapping](#)

- *Automatic Selection of Exposure, Exam or Exposure group*

## Basic Mapping

Purpose: correctly map the RIS data structures to NX data structures so that at run-time of NX the patient and exam data from RIS are correctly received.

During creation of the RIS device in the NX Service and Configuration Tool, you had to select a pre-defined mapping in this dialog:

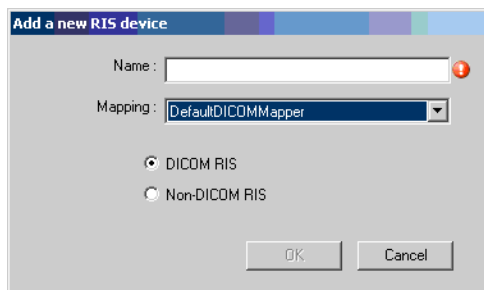

**Figure 76: NX Service and Configuration Tool - Add Ris dialog box**

The following steps explain how to change the mapping for this RIS device.

Go to the ‘mapped fields’\‘unmapped fields’ sections in the RIS setup page to change the mapping.

- “The Mapped Fields Section”
- “Fields”
- “Buttons”
- “The Unmapped Fields Section”
- “Available Default Mappings”

## Topics:

- *The Mapped Fields Section*
- *Fields*
- *Buttons*
- *The Unmapped Fields Section*
- *Available Default Mappings*

### The Mapped Fields Section

This section defines the mapping.

On the left you will see the RIS fields, at the right the internal NX fields. One row represents one mapping.

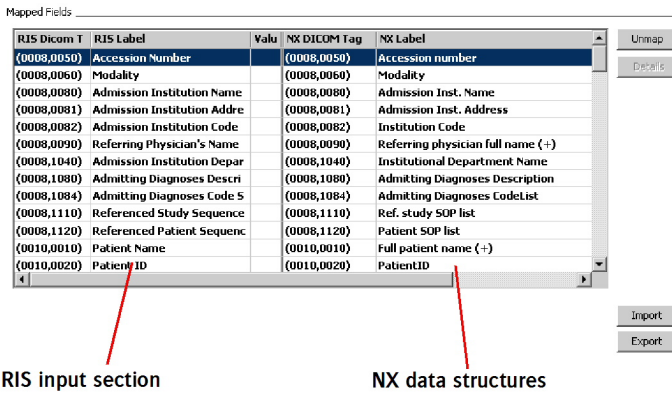


Figure 77: NX Service and Configuration Tool - RIS mapping

**Fields**

- Simple fields

It is possible to map a simple RIS field on a simple NX field.

For example: patient ID



Figure 78: 20121129 - RIS mapping

- Sequences

Some fields in these tables refer to sequences. They are typically indicated by the word 'sequence' or 'list' at the end.

It is possible to map a sequence to an NX sequence

For example:



Figure 79: NX Service and Configuration Tool - RIS mapping

It is also possible to map a single field to a sub-field of the 'protocol code' sequence.

For example:



Figure 80: NX Service and Configuration Tool - RIS mapping

In this case, do NOT also map the sequence itself as the results are unpredictable.

The sub fields of a sequence have the same NX DICOM tag as the sequence itself. E.g.

0040,0008	Scheduled protocol code sequence	<p>This is the sequence</p> <p>These are the subfields of the sequence</p>
0040,0008	protocol code value	
0040,0008	protocol code scheme designator	
0040,0008	protocol code scheme version	
0040,0008	protocol code meaning	

- Person Names

For person names, there is a field for the whole name and there are fields for the sub-parts of the name.

For example, the whole name:

(0010,0010)	Patient Name
(0010,0020)	Patient ID

**Figure 81: NX Service and Configuration Tool - RIS mapping**

For example, the sub-fields:

(0010,0010)	Patient first name
(0010,0010)	Patient full name
(0010,0010)	Patient name prefix
(0010,0010)	Patient middle name
(0010,0010)	Patient name suffix
(0010,0010)	Patient last name

**Figure 82: NX Service and Configuration Tool - RIS mapping**


You can choose which to map (the whole name or one or more of the sub-fields). It is not advised to use both as the results are unpredictable.



*Note: This also applies to Referring physician, patient mother, requesting physician, performing physician, orderer, ...*

### Buttons

Unmap	Remove a mapping from the mapped fields. It will be added to the unmapped fields
Details	For displaying the received values of a 'sequence' field. E.g. when selecting the line containing '0008:0082' and pressing the details button, the following window will appear showing all received data for this sequence field:

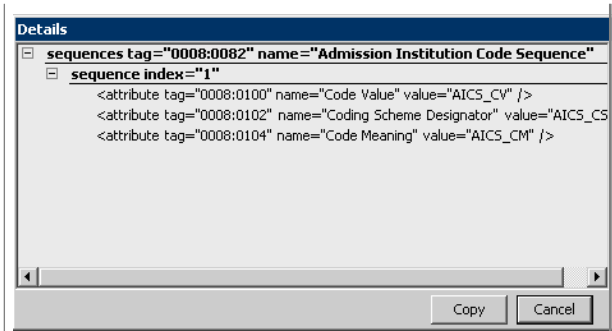

**Figure 83: NX Service and Configuration Tool - RIS mapping**

Import	Import a mapping from file. Current mappings will be lost.
Export	Export current mapping to file.

In case of a DICOM RIS: only the fields that are mapped will be requested from the RIS during the DICOM modality worklist query.

As a RIS may have problems with some attributes, leave them out from the mapping to avoid these problems.


Do NOT unmap the 7 mandatory DICOM attributes (in case of a DICOM RIS):

- Station AE Title list
- Scheduled start date
- Scheduled start time
- Modality
- Performing physician full name (+)
- Full patient name (+)
- PatientID

### The Unmapped Fields Section

This section lists:

- at the right side: all known NX fields that are not part of the actual mapping
- at the left side: a working area to add new fields ('Add unmapped field' button) or for fields that get unmapped from the 'mapped fields' section

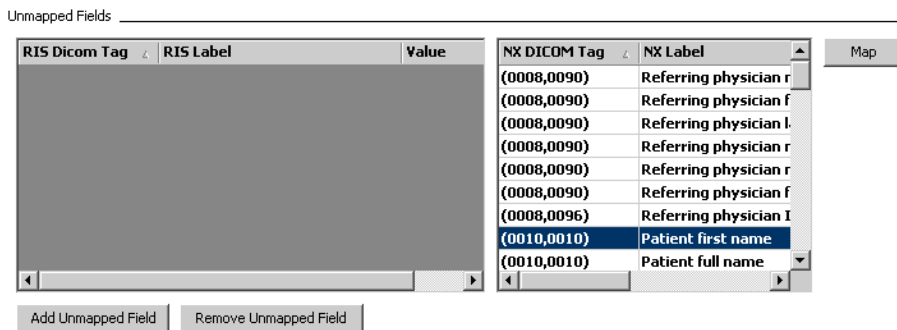

**Figure 84: NX Service and Configuration Tool - RIS mapping**

Map	Adds current selection to the mapping.
Add unmapped field	Allows to enter a new field to the unmapped field list. By supplying the DICOM tag and label, a new unmapped field will be created. This unmapped field can then be mapped to the NX DICOM tag in a further step.
Remove unmapped field	Allows to remove a field from the unmapped field list.

### Available Default Mappings

- For DICOM RIS:

These can also be used for a non-DICOM RIS!

Default DICOM mapper	A fixed list of +/- 50 attributes. This is the same list as what was queried in NX 1.0 but 'problem' attributes left out (E.g. 0040, 000B). Select this mapping to view the contents.
Extended DICOM mapper	A fixed list of +/-96 attributes. Select this mapping to view the contents.
Extended DICOM mapper 2006	A fixed list of +/-95 attributes. Select this mapping to view the contents.

- For non DICOM RIS:

non DICOM V0 protocol	Select this mapping to view the contents.
non DICOM V1 protocol	Select this mapping to view the contents.

non DICOM V2 protocol	Select this mapping to view the contents.
-----------------------	---



*Note: These can also be used for a DICOM RIS.*

- Buttons in the RIS mapping section

Query RIS	Performs a DICOM Modality Worklist Query towards the RIS with given settings. The query uses the configured mapping.
Restore defaults	Allows to load a default mapping, all current mapping will be lost.

## More Details on Mapping


### Topics:

- [Person Name Representation](#)
- [Red Lines](#)

#### Person Name Representation

NX will internally resolve some attributes to the correct 'Person Name Representation', depending on its setting in 'User Interface Configuration – General settings'.

- If there is no “+” at the end of the attribute in the NX Label column, then NX will adapt the person name representation to the representation configured in the User Interface Configuration section of the NX Service and Configuration tool.

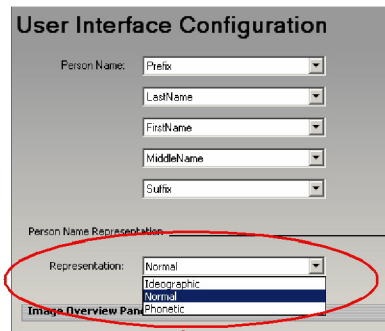

Performing Physician Full name Normal  
 or  
 Performing Physician Full name Ideographic  
 or  
 Performing Physician Full name Phonetic

'Performing Physician Full name'  
 (without the "+" at the end)

**Figure 85: NX Service and Configuration Tool - RIS mapping - Person Name Representation**

- If there is a "+" at the end of the attribute in the NX label, all Person Name Representations will be sent.

For example:

Mapped Fields

RIS Dicom T	RIS Label	Valu	NX DICOM Tag	NX Label
(0040,0001)	Scheduled Station AE title		(0040,0001)	Station AE-title list
(0040,0002)	Scheduled Procedure Step S		(0040,0002)	Scheduled start date
(0040,0003)	Scheduled Procedure Step S		(0040,0003)	Scheduled start time
(0040,0006)	Scheduled Performing Physi		(0040,0006)	Performing physician full name (+)
(0040,0007)	Scheduled Procedure Step D		(0040,0007)	SPS Description
(0040,0008)	Scheduled Protocol Code Se		(0040,0008)	Scheduled Protocol code Seq.
(0040,0009)	Scheduled Procedure Step I		(0040,0009)	SPS ID
(0040,0008)	Scheduled Performing Physi		(0040,0008)	Performing physician ID
(0040,0010)	Scheduled Station Name		(0040,0010)	Station name list
(0040,0011)	Scheduled Procedure Step L		(0040,0011)	Location
(0040,0012)	Pre-Medication		(0040,0012)	Pre-Medication
(0040,0020)	Scheduled Procedure Step S		(0040,0020)	SPS Status
(0040,0400)	Scheduled Procedure Step C		(0040,0400)	SPS comments

'Performing Physician Full name' (+)

Performing Physician Full name Normal  
 and  
 Performing Physician Full name Ideographic  
 and  
 Performing Physician Full name Phonetic

**Figure 86: NX Service and Configuration Tool - RIS mapping - Person Name Representation**

**Related Links**

[Person Name Representation](#) on page 208

## Red Lines

After a query, some mapping lines may be shown in red. This means that the type of the value received from the RIS does not match the type of the configured field, change this.

Mapped Fields

RIS DICOM Tag	RIS Label	Value	NX DICOM Tag	NX Label
(0000,1001)	None	Unable to read obje	(0020,0008)	Study instance uid
(0008,1001)	Name	a63934010510101	(0008,0050)	Accession number
(0008,0090)	ReferringPhysician		(0008,0090)	Referring physician full n
(0010,0020)	Patient ID		(0010,0020)	PatientID
(0010,0030)	Patient Birth Date		(0010,1030)	Patient birthdate
(0010,0040)	Patient Sex		(0010,0040)	Patient Sex
(0019,2001)	Patient First Name		(0010,0010)	Patient first name
(0019,2002)	Patient Last Name		(0010,0010)	Patient last name
(0020,4000)	Scheduled Procedure		(0040,0400)	SPS comments

Figure 87: NX Service and Configuration Tool - RIS mapping - Red Lines

It can also mean that the value cannot be interpreted, i.e. values which are defined by DICOM and which are mapped to enums

## Automatic Selection of Exposure, Exam or Exposure group



*Note: A wrong specification of protocol codes for the exposure group may lead to insufficient image quality.*

This section explains automatic exposure (or exam or exposure group) selection in NX from the code values coming from RIS (query).


When automatic exposure (or exam or exposure group) selection is required, then the NX attribute 0040,0008 'Protocol code value' needs to be filled in correctly with the right data coming from the RIS. This field does the magic of automatically selecting at NX run time of:

- an exposure
- or an exam
- or an exposure group

Two configuration actions are required to enable automatic selection of exposure, exam or exposure group:

1. Mapping the correct RIS data field to NX field 0040,0008 'Protocol code value'. Which fields can be mapped, is described in "Mapping the Protocol code value". How to map RIS fields is described in "The Mapped Fields Section".
2. Linking protocol code values to the right exposure, exam or exposure group. This is done in the 'Link protocol code' page.

Overview

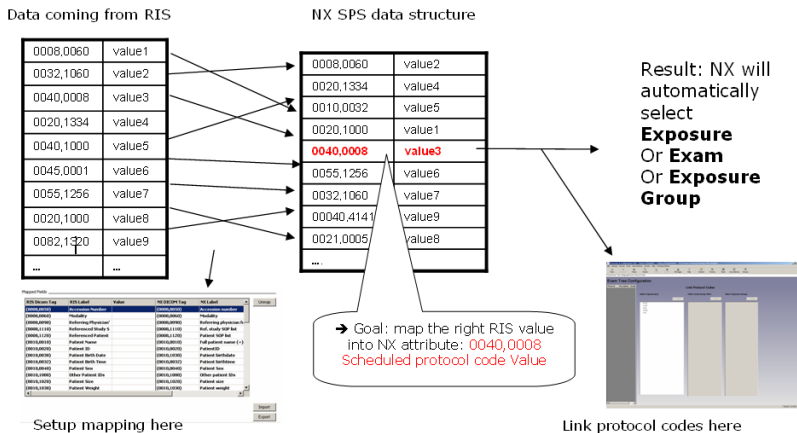

**Related Links**

[Mapping the Protocol code value](#) on page 124

[The Mapped Fields Section](#) on page 116

**Topics:**

- [Mapping the Protocol code value](#)
- [Japanese Protocol Codes](#)

**Mapping the Protocol code value**

0040,0008 Scheduled protocol code sequence is a sequence with 4 sub-fields:

- Protocol code value.
- Protocol code scheme designator.
- Protocol code scheme version.
- Protocol code meaning.

In the NX mapping list you will find these fields all having the same tag: 0040,0008, even the sequence itself:

0040,0008	Scheduled protocol code sequence
0040,0008	Protocol code value
0040,0008	Protocol code scheme designator
0040,0008	Protocol code scheme version
0040,0008	Protocol code meaning

Only 'protocol code **value**' needs to be filled in correctly with data from the RIS! This can be obtained in 3 ways:

- Map the complete **0040,0008 RIS sequence** to the NX 0040,0008 Scheduled protocol code **sequence**.

This can be done as both are ‘sequences’ (and you can only map a sequence to a sequence).

or

- Map the complete **0032,1064 RIS Requested procedure code sequence** to the NX 0040,0008 Scheduled protocol code **sequence**.


This can be done as both are sequences (and you can only map a sequence to a sequence). This mapping is typically required for connecting Agfa’s Connectivity Manager.

or


- Map the custom (string) field where the RIS stores the protocol code value to NX 0040,0008 protocol code value.

Overview:


### 1. Map complete 0040,0008 RIS sequence to

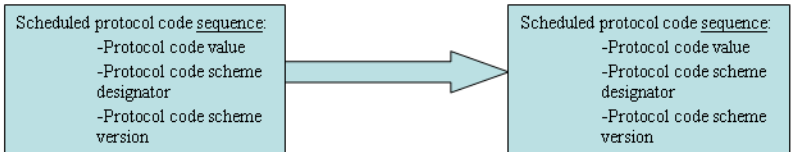

### 2. Map complete 0032,1064 RIS sequence to

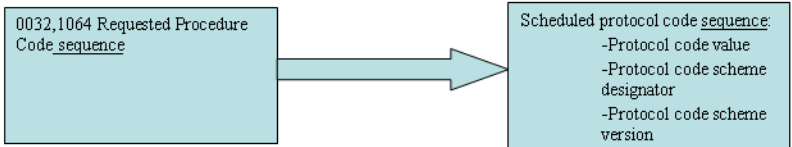

### 3. Map any other (string) field to

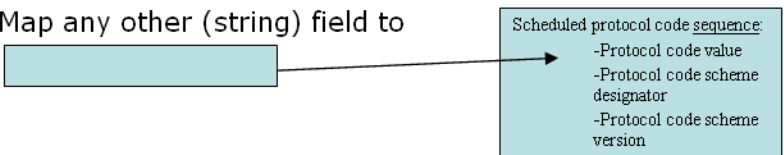

## Japanese Protocol Codes

For Japanese protocol codes, it is not enough to map to 0040,0008 Protocol code value. Two extra attributes must be used, separated by ^ when configuring protocol codes in the examtree, see JJ1017 guidelines under “Configuring Main RIS Settings”.

For examtree configuration:

protocol code value = Scheduled Procedure Step Sequence code value ^ Concept Code Sequence Code Value of target Region ^ Concept Code Sequence Code Value of Imaging Direction

## Related Links

[Configuring Main RIS Settings](#) on page 109

## Configuring the X-Ray Device

---

This type of device is only available when one of the following licenses is enabled:

- IDIS1 connection
- XRG connection for mammo
- DR workflow




*Note: Only enabling the DR Workflow license will give the user NO ability to add a new X-ray device or configuring it (for DR also the IDIS license should be enabled).*

### Topics:

- [Configuring an X-Ray Device](#)
- [Configuring a DR Detector](#)
- [Configuring the Generator Settings](#)
- [Configuring the Retrofit Box Settings](#)
- [Configuring the DR Image Recovery Exposure Type](#)
- [Configuring the Room Settings](#)

## Configuring an X-Ray Device

To configure the X-Ray Device, click **New**.

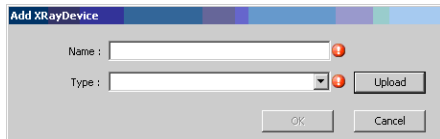

**Figure 88: Add X Ray Device dialog.**

Name	Enter a nickname
Type	<p>Select the correct model file, matching the X-Ray Device manufacturer and type. If a DR Detector is connected to the NX, a dedicated model file for DR support must be loaded.</p> <p>If none are available, install XRDI software first.</p> <p>These model files are only installed on the system after installing the XRDI software (which comes separate from NX).</p> <p>Further, for each model a specific license must be available in the license file (ALF).</p>

The content of the X-Ray device screen depends further on the loaded type. Typically, only connection related parameters can be entered and a test button is foreseen.

To delete the X-Ray Device, click **Delete**. All modality settings in the exam tree configuration will be cleared.


## Configuring a DR Detector

To configure a DR Detector:

1. Go to the Detector Settings pane in the X-Ray Device Configuration screen and click Add.
2. Select the correct model file, matching the DR Detector manufacturer and type.

Model files are available in C:\Agfa\Healthcare\NX\Bin  
\XRyDeviceModels\DRPanelModels\

In the Detector Settings pane, a new tab is created that contains the settings for the DR Detector.

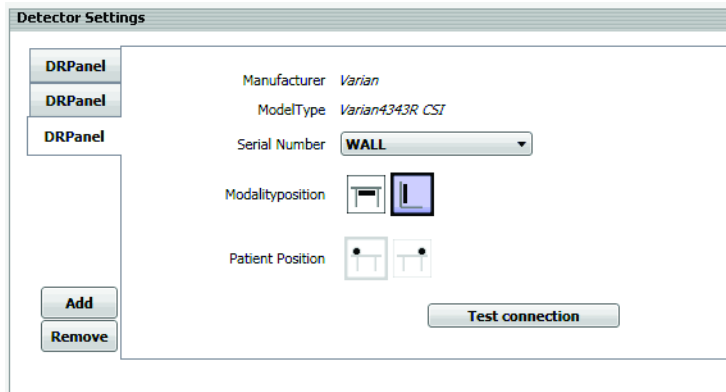

**Figure 89: X-ray Device Configuration screen - Detector Settings pane.**

3. Identify an installed DR Detector by selecting the Serial Number.  
If none are available, install the DR Detector driver software first.


**Table 1: DR Detector Settings**

Modality Position	The DR Detector can be assembled in the table or in the wall stand or used for free exposures.
Patient Position	A table detector can be configured for 'head left' or 'head right' patient positioning.
Nickname	A portable DR Detector can be given a nickname to identify it among other portable DR Detectors.

## Configuring the Generator Settings

To configure the generator settings:

1. Go to the Generator Settings pane in the X-Ray Device Configuration screen.

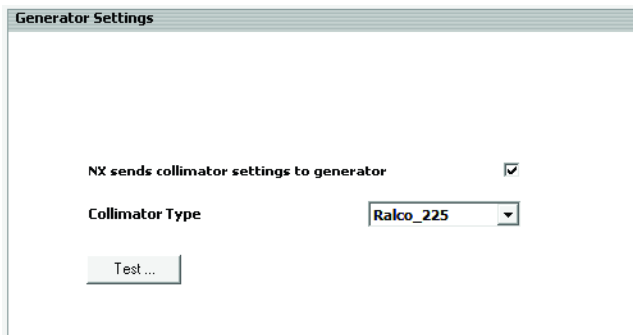

**Figure 90: Generator Settings**

2. Define:
  - If NX sends collimator settings to the generator.
  - The collimator type.

## Configuring the Retrofit Box Settings

If the configuration contains a Retrofit Box or DR Detector Router, apply the correct settings:

1. Go to the Retrofit Box Settings pane in the X-Ray Device Configuration screen.

	Port 1	Port 2	Port 3	Port 4	Virtual Port A	Virtual Port B
Default	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
TABLE	<input type="checkbox"/>	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>

**Figure 91: Retrofit Settings**

2. Define these settings:

- whether the configuration contains a Retrofit Box or DR Detector Router
- whether it is configured as a router

If the exposure button is connected to the Retrofit Box, it is not configured as a router and a prepdelay must be configured.

- the prepdelay

When pushing the exposure button, the Retrofit Box starts the prep cycle on the X-ray generator. After a configurable delay the exposure cycle is started.


- the ports to which the DR Detectors are connected.

## Configuring the DR Image Recovery Exposure Type

Define the settings to apply when a DR image is received that cannot be linked to a listed exposure. An Age group, examination group and Exposure type will have to be defined.

To configure the DR image recovery exposure type:

1. Go to the DR Recovery Procedure pane in the X-Ray Device Configuration screen.

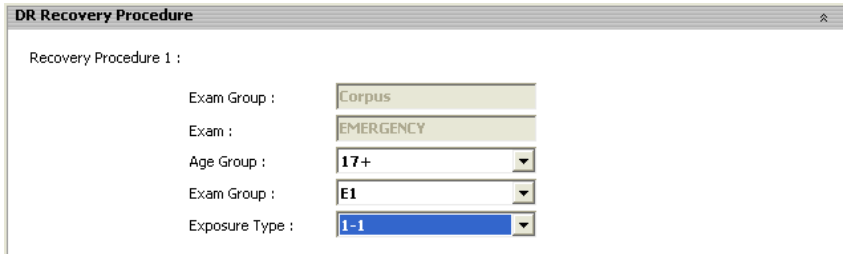

The screenshot shows a window titled "DR Recovery Procedure" with a close button in the top right corner. Inside the window, the text "Recovery Procedure 1 :" is displayed. Below this, there are five configuration items, each with a label and a dropdown menu:

- Exam Group : Corpus
- Exam : EMERGENCY
- Age Group : 17+ (with a downward arrow)
- Exam Group : E1 (with a downward arrow)
- Exposure Type : 1-1 (with a downward arrow)

2. Define an Age group, examination group and Exposure type.

## Configuring the Room Settings

The Room settings reflect the physical setup of the FLFS equipment and are only available for the service user.

To configure the X-Ray Device Room settings

1. Go to the Room Settings pane in the X-Ray Device Configuration screen.

Maximum Longitudinal Patient Movement	▼	0	▲
Maximum Transverse Patient Movement	▼	0	▲
Vertical Detector Top Height	▼	0	▲
Vertical Detector Bottom Height	▼	0	▲
Stitching Grid To Vertical Detector distance	▼	0	▲

**Figure 92: Room Settings**

2. Define:
  - the distance between the detector and the stitching grid of the DX Full Leg Full Spine stand
  - the maximum values for horizontal and vertical patient movement
  - the vertical detector top height, which is the height of the top edge of the detector in its highest position during a FLFS-examination.
  - the vertical detector bottom height, which is the height of the bottom edge of the detector when the detector is in its lowest position during a vertical FLFS-examination.

## Configuring Rooms

---

### Topics:

- *General*
- *Configuring Workstations for Central Administration*

## General



*Note: The Configure Rooms functionality is specific for the Central Monitoring System.*



*Note: Some settings in the NX Service and Configuration Tool for the Central Monitoring System may be greyed out because they are not relevant to the Central Monitoring System.*

This screen allows configuring the NX workstations that are connected to a Central Monitoring System.


The ‘configured rooms’ table lists all NX workstations which will be connected to this CMS.

Only NX workstations belonging to the same NX software family can be connected (they have the same main version numbers).

For example:

- Allowed connection is NX2.0.6805 and NX2.0.6805 SU2
- Not allowed connection is NX2.0.6805 and NX3.0.2900

<p>Scan button</p>	<p>Performs a network scan for connected NX workstations (the NX back end application must be running on the in-room PCs).</p> <p>From the result dialog, NX workstations can be added to the ‘configured rooms’ table.</p>
--------------------	---

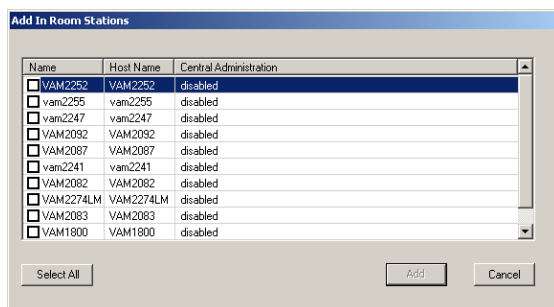

**Figure 93: NX Service and Configuration Tool - Scan button for In Room Stations**

The 'Central Administration' column indicates whether the Dose and RRAP statistics are archived centrally or not.

On an in-room NX this is configured in Workflow management.

Central Administration \_\_\_\_\_  
 Store dose and RRAP statistics centrally

**Figure 94: NX Service and Configuration Tool - Central Administration check box**

New button	To manually add a new NX
Test connection button	Test connection with selected NX
Remove button	Remove an NX from the 'configured rooms' table
Store button	Adds values entered manually in 'name' or 'hostname' to the 'configured rooms' table
Name	To edit\enter a nickname of an NX
hostname	To edit\enter a hostname of an NX

## Related Links

[Identification General](#) on page 52

## Configuring Workstations for Central Administration

This is a setting for NX-in-room workstations which are part of a Central Monitoring System. When Central Administration is enabled, repeat reject analysis statistics and dose monitoring statistics will be available on the Central Monitoring System, and these functions will be disabled on the NX workstation.

Procedure:

1. The NX workstation of which you want to have the administration centrally managed, must be configured for Central Monitoring on the Central Monitoring System.
2. On the NX Workstation of which you want to have the administration centrally managed, open the NX Service and Configuration Tool and go to “Workflow Management” .
3. If it is collapsed, open the Identification pane and select the Central Administration check box.

From this moment, managing repeat reject statistics and managing dose monitoring statistics will only be possible on the Central Monitoring System.

The Main Menu entries for repeat reject analysis and dose monitoring statistics will be disabled on the in-room NX workstations.



*Note: It is not necessary to configure all NX workstations in the Central Monitoring System for central administration.*



*Note: It is not possible to manage Repeat Reject statistics locally and Dose Monitoring statistics centrally on the same workstation (or vice versa).*



*Note: When activating Central Administration, data that were already on the local workstation are transferred to the Central Monitoring station and vice versa.*



*Note: A CMS configured to work with Exposure Index can NOT communicate with a workstation that is configured to operate with LGM and vice versa.*

# Configuring Security Issues

---

## Topics:

- *General Security Settings*
- *Managing Users*
- *Managing Licenses*
- *Service Log In*
- *Deleting Examinations*

## General Security Settings

---

### Topics:

- [\*Configuring SSL Settings\*](#)
- [\*Configuring Audit Log Settings\*](#)

## Configuring SSL Settings

Secure DICOM means that DICOM connections will be setup over SSL (Secure Sockets Layer).

Refer to your local service representative for advise on configuring the system and setting up the required certificates for the NX workstation and the connected devices.

## Configuring Audit Log Settings

Audit logging allows NX to send short messages to an Audit log server on the network. These messages indicate some actions done on NX.

### Topics:

- [Audit Log General Settings](#)
- [NTP Settings](#)

### Audit Log General Settings

Audit log server settings	
Hostname IP address IP Stack	Fill in either hostname and IP Stack or IP address (IP Stack detected automatically).
Port number	Network port number the audit log server is listening on
Fallback log file settings	
Maximum file size	When the audit Log server is unreachable, NX stores the audit logs in a file. This file should be on the local filesystem. When the configured file size is reached, the oldest loggings are removed (FIFO principle).
Location	
Send log file	Use the Send Log file button to manually send the contents of the fallback log file to the Audit Log server when it is back online.
Time zone settings	
Time zone	Specifies the time indication in the audit logs, according Local time zone or UTC

## NTP Settings

NTP: Network Time Protocol, used to retrieve the current time from a network time server. Allows NX to synchronize the time in the audit loggings with the time on the NTP server.

Hostname	Fill in either hostname and IP Stack or IP address (IP Stack detected automatically).
IP address	
IP Stack	
Port number	The port number the network NTP server is listening on for the NTP protocol.

## Managing Users

---

### Topics:

- [General](#)
- [Assigning User Roles](#)

## General

With the NX Service and Configuration Tool you can configure users. Typically, users are imported from the Windows domain of the hospital. The users are displayed in a list view (at the left hand side of the central viewing area). Details of the selected user are displayed within the body of the central viewing area.

If you select a user, the roles of this user will be displayed in the Role pane.

In this window you can:

- Define new users
- Delete users
- Manage roles. When clicking this last button, a separate User Role Configuration page is shown.

## Assigning User Roles

The User Role Configuration page is dedicated to the functionality related to user roles and associated operations.

The user roles are displayed in a list view (at the left hand side of the central viewing area) and a detailed overview of the users assigned to this role and the tasks related with this role are displayed within the body of the central viewing area.

If you change the roles of the user logged in, the NX Service and Configuration Tool reflects the changes in the role of the user logged in immediately. For example, if you are logged in as “crservice” and you change the role of crservice, changing the user interface will be impossible from that moment.

### Assigning user roles to users in a group

1. Add the group to the NX configuration.  
Proceed as for adding a user and select the **Group** option in the **Add account** dialog
2. Assign roles to the group instead of the individual users.

All users in the group share the assigned roles.

## Managing Licenses

---

To manage licenses for NX, you must perform a number of actions in two separate environments, as described in the following sections.

- “Managing Licenses in the License Manager” .
- “Managing Licenses in the NX Service and Configuration Tool” .
- “Trial Licenses”




*Note: it is strongly advised to always use the License Manager to check the status of the licenses instead of the licenses screen in the NX Service and Configuration Tool !*

### Topics:

- [Managing Licenses in the License Manager](#)
- [Managing Licenses in the NX Service and Configuration Tool](#)
- [Trial Licenses](#)

## Managing Licenses in the License Manager

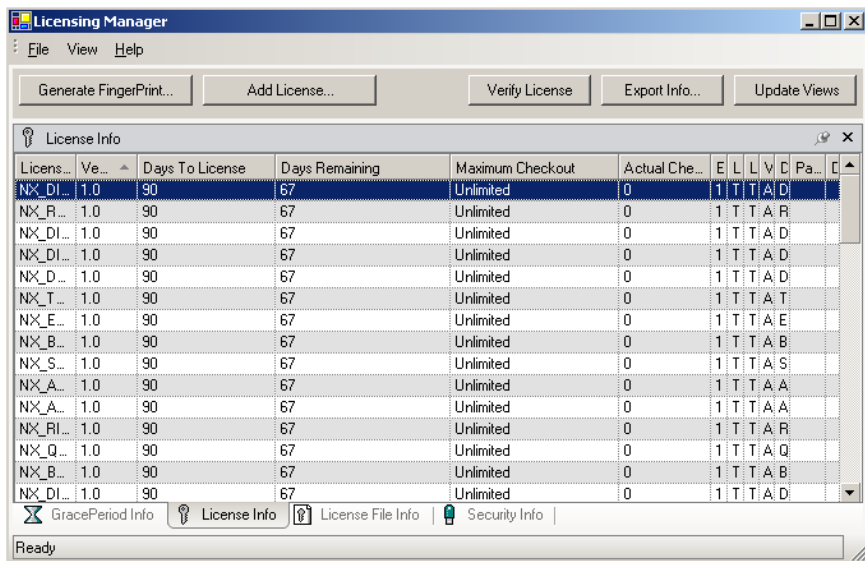

**Figure 95: License Manager**

Run the License Manager via : START MENU > AGFA > SERVICE > License Manager.

Use the License Manager to check:

- Installed licenses
- remaining days valid
- whether the system is running in grace or not
- dongle info
- verification of license versions
- ...

The licenses screen in the NX Service and Configuration Tool is only to be used in exceptional situations !

The licenses shown are technical licenses (similar as in the License Manager). Technical licenses are typically grouped in an ABC code package (=option or starter pack which is available for sale).

Each license has a version number.

Eg. 1.0 for license NX\_QA\_TOOLS.

This version number can change over different NX releases.

The version number must be correct for the functionality behind the license to be useable in NX. The License Manager indicates if there is a license number mismatch.

## Managing Licenses in the NX Service and Configuration Tool

On an online NX, the NX Service and Configuration Tool will not startup if no ALF (license file) is loaded.

On an NX workstation, the NX Service and Configuration Tool lists all NX licences that are available in the ALF file (license file). The NX Service and Configuration Tool will not startup if no ALF is loaded in the License Manager.

No licenses from other products are shown in here (eg. from XRDI or AutoQC<sup>2</sup>).

The NX Service and Configuration Tool allows to disable licenses and enable them later. These actions do not affect the loaded ALF.

Enabling/disabling licenses has an immediate effect on the other screens of the NX Service and Configuration Tool (the corresponding functionality will be shown or not).


In an offline situation, no ALF is required and the NX Service and Configuration Tool will list all existing NX licenses. You can disable licenses that will not be present on the online NX in order to represent the online situation as much as possible.



*Note: The NX Service and Configuration Tool does NOT check if there is a license version number mismatch. If the license version number is not correct, the corresponding functionality in NX will not be useable, although it is configurable in the NX Service and Configuration Tool. Use the License Manager to check for version mismatches.*

## Trial Licenses

NX will display the status of the trial (demo) licenses every 6 hours (plus at startup):

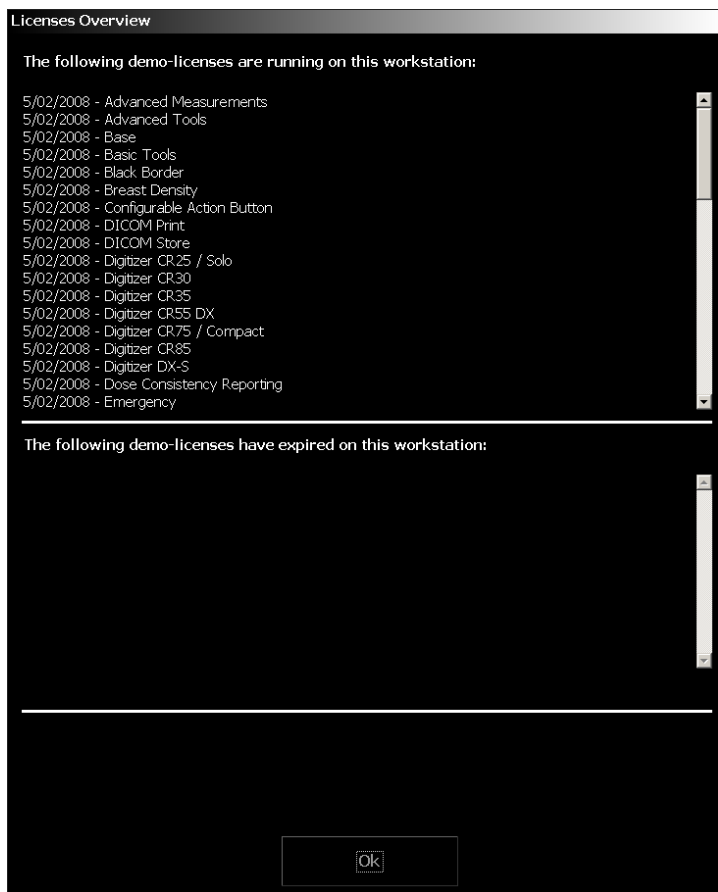

**Figure 96: NX - License Overview at startup**

The expire date of trial licenses will be indicated.

Expired demo-licenses remain active until the next reboot of the NX Workstation

## Service Log In


In case no Service Engineers are defined in Manage Users and Manage user roles, this login dialog allows you to enter a fixed username\password. Then it becomes possible to configure a service engineer in Manage Users and Manage user roles (typically yourself).

## Deleting Examinations

---

Allows to force-delete exams in NX.

This functionality should be used with care!

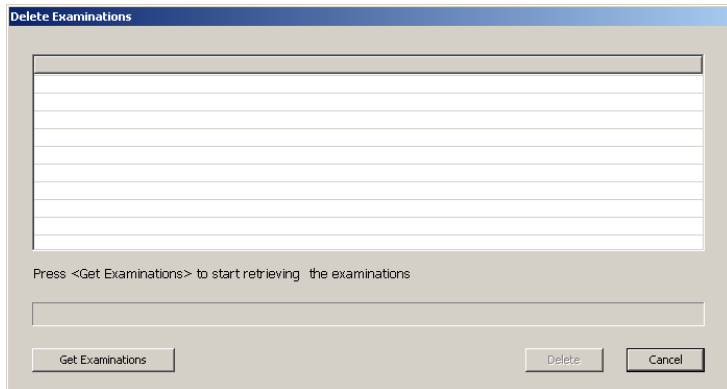

Click the 'Get Examination' button to load all exams in NX. You can select and delete them afterwards.



*Note: The selected exams are permanently removed from the system without checking first whether they are closed, printed, archived or exported. unrecoverable image loss can happen if an exam is deleted before the images are archived, printed or exported.*

This functionality should only be used when all normal ways to remove an exam fail (automatic cleanup by NX, deletion via the NX main menu, ...)

# Configuring the Examination Tree

---

## Topics:

- *Main Window*
- *Configuring Examination Groups*
- *Configuring Exposure Types*
- *Configuring Exposure Groups*
- *Managing Protocol Codes*


## Main Window

---

### Topics:

- *Introduction*
- *Main Screen Functions*
- *Partial Loading of an Exam Tree*
- *Tips & Tricks*

## Introduction

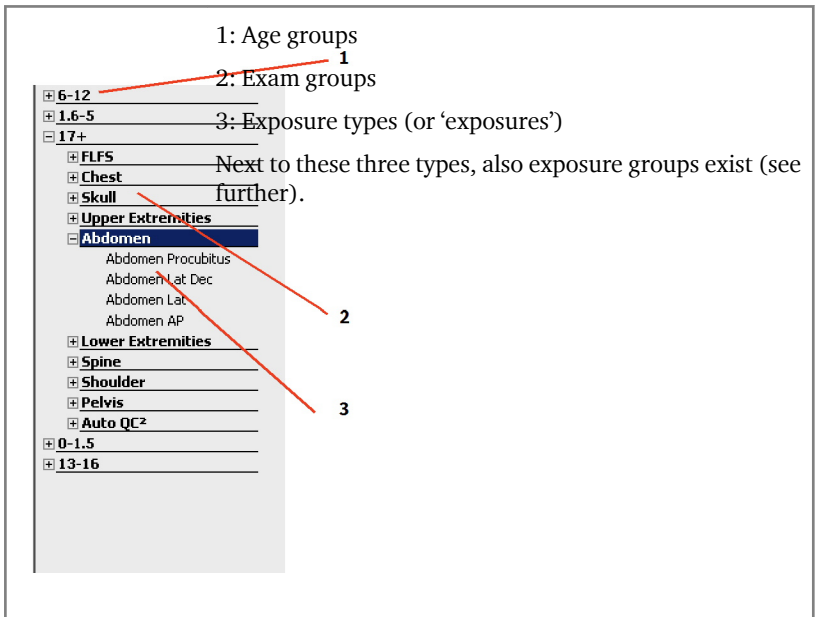

### Topics:


- *Age Groups*
- *Exam Groups*
- *Exposure Types (or 'Exposures')*
- *Exposure Groups*

### Age Groups

Age groups are used to group all the exam groups for a particular age.

Following age groups exist: 0-1.5 year, 1.6-5 year, 6-12 year, 13-16 year, 17+ years.

Age groups themselves are fixed and not configurable by the user. This means that every NX system will have the same age groups boundaries. The first four age groups - the Pediatric age groups - will only be visible when the system has the pediatric license enabled. Otherwise, only the age group 17+ year will be visible.

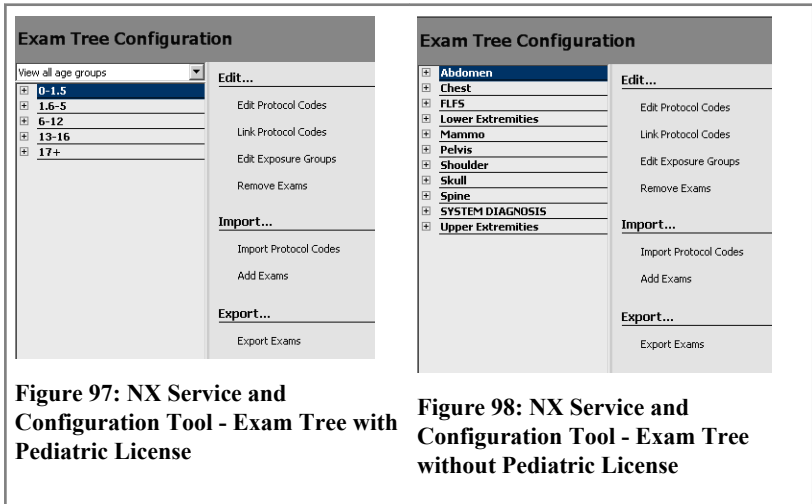

## Exam Groups

Exam groups group all exposures that are clinically related. Example: Upper extremities, Chest, Skull, Lower extremities, Abdomen, Spine. Each Exposure type can only be part of one Examination group. Every age group will have the same exam groups. E.g. If one age group contains the exam group Chest, all age groups will contain this exam group.

Exposure types for test images will be stored in a special test images exam group ('System diagnostics'). These are partially editable by the Service Engineer.

## Exposure Types (or 'Exposures')

An exposure type is the central element in the exam tree. It contains predefined values for acquisition of an image.

### Related Links

[Configuring Exposure Types](#) on page 162

## Exposure Groups

next to the three levels (age groups, exam groups, exposure types) that make up an NX exam tree, there are also exposures groups.

### Related Links

[Configuring Exposure Groups](#) on page 184

## Main Screen Functions

### Topics:

- [Editing](#)
- [Exporting](#)
- [Adding new Exams, Exposures or Exposure Groups](#)
- [Finding and replacing](#)
- [Edit exposure modality settings](#)

### Editing

Edit protocol codes	Refer to “Editing Protocol Codes”
Link protocol codes	Refer to “Linking Protocol Codes”
Edit exposure groups	Refer to “Configuring Exposure Groups”
Remove exams	Removing an exam group: removes it for in all age groups! You cannot undo this!

### Related Links

[Editing Protocol Codes](#) on page 199

[Linking Protocol Codes](#) on page 195

[Configuring Exposure Groups](#) on page 184

### Exporting

Export exams	Just exports the selected exams (including their contents) to an xml file (for all Age Groups).
--------------	---

### Adding new Exams, Exposures or Exposure Groups

Add new exam	To create a new exam group. This new exam group will be created for all Age groups.
Add new exposure	To create a new exposure (can be put in any exam group).
Add new exposure group	To create a new empty exposure group. You can configure it further in “Configuring Exposure Groups” .

### Related Links

## Configuring Exposure Groups on page 184

### Finding and replacing

This screen allows you to selectively change attributes of exposures.

At the left side, search criteria can be entered. Applying the Find button queries the whole exam tree search for exposures that adhere to the given search criteria. The query results are shown at the bottom.

**Find...**

Age Group: 17+ Exam Group: -- Select an exam group --

Application: General radiology Body Part: -- Select a body part --

**General Settings**

View Position:  AP  PA  LL  RL

Speed Class:  12  18  25  37

Cassette Orientation:  Landscape  Portrait

Image Laterality:  R  L  U  B

Erasure Dose:  100  300  750

Scale Mode:  Scale to fit  True size

**Processing Settings**

Collimation: -- Select collimation -- Collimation Border:  On  Off

**Destinations**

Printer: -- Select a printer -- Print Automation:  On  Off

Sheet Size: -- Select a sheet size -- Archive Automation:  On  Off

Print Automation on image arrival:  On  Off

Archive Automation on image arrival:  On  Off

**Find**

**Replace with...**

**General Settings**

View Position: -- Select a position -- Speed Class: -- Select a speed class --

Cassette Orientation: -- Select an orientation -- Erasure Dose: -- Select an erasure dose --

Image Laterality: -- Select a laterality -- Scale Mode: -- Select a scale mode --

Target Exposure Index: NONE

**Processing Settings**

Collimation: -- Select a collimation -- Collimation Border: -- Select a border --

Package: -- Select --

MCE Image Requested: -- Select MCE Image Request --

**Destinations**

Printer: -- Select --

Sheet Size: -- Select --

Print Automation: -- Select print automation --

Archive Automation: -- Select archive automation --

Additional Destination(s): -- Select Additional Destinal -- -- Select Additional Destinal --

**Replace**

**Result List**

You have searched for: Age group: 17+; Application: General radiology; View Positions: PA; Orientations: Portrait;

Age Group	Exam Group	Application	Body Part	Exposure	View Positi...	Orientation	Laterality	Speed Class	Erasure D...	Scale Mode	
<input checked="" type="checkbox"/>	17+	Lower Ext...	General ra...	Knee	Knee Cond...	PA	Portrait	U	200	100	Scale to fit
<input checked="" type="checkbox"/>	17+	Abdomen	General ra...	Abdomen	Abdomen	PA	Portrait	U	200	100	Scale to fit
<input type="checkbox"/>	17+	Skull	General ra...	Skull	Skull PA	PA	Portrait	U	200	100	Scale to fit
<input type="checkbox"/>	17+	Skull	General ra...	Skull	Orbita PA	PA	Portrait	U	200	100	Scale to fit
<input checked="" type="checkbox"/>	17+	Skull	General ra...	Skull	Sinus PA	PA	Portrait	U	200	100	Scale to fit
<input checked="" type="checkbox"/>	17+	Upper Ext...	General ra...	Shoulder	Humerus Y	PA	Portrait	U	200	100	Scale to fit
<input checked="" type="checkbox"/>	17+	Shoulder	General ra...	Shoulder	Scapular Y	PA	Portrait	U	200	100	Scale to fit

**Figure 99: NX Service and Configuration Tool - Find and Replace**

At the right side, you can enter new values for certain exposure attributes. By clicking the Replace button, the exposures in the result list are updated with the new values. To store the changes, click the Commit button, to undo the replace, click the Cancel button.



*Note: Application type is a mandatory field in the Find pane. A Find and Replace operation is always limited to the context of one application type.*

### Editing the Target Exposure Index setting

To update the Target Exposure Index for the matching exposure, enter a new value (one digit after the decimal point).

To clear the Target Exposure Index for the matching exposures, leave the field blank.

To leave the Target Exposure Index unchanged, enter 'NONE'.

## Edit exposure modality settings

This screen allows you to selectively change modality settings of exposures.

The screenshot shows the 'Exam Tree Configuration' window. At the top is a table with columns for Exam, Exposure, Study, Modality, Detector, and various exposure parameters like mAs, mA, max mA, and AEC. Below the table is a settings pane for the selected exposure. The settings pane includes sections for General settings, ViewName, Modality position, Detector Modality, Focus, Grid, and Position settings. A red arrow labeled '1' points to the table, and another red arrow labeled '2' points to the settings pane.

### 1. Grid view

- Each row represents an exposure
- Each column contains the value for an exposure setting

### 2. Settings pane for the exposure of the selected row

**Figure 100: Edit exposure modality settings**

- Filter the exposures by selecting a value in the drop-down selector on the header title row of each column.
- Select a row to edit the modality settings in the settings pane.
- Select multiple rows using the shift or control keys and right click a column to apply the same setting to all selected rows.

**Table 2: Cell color indication**

Cell	Color	Meaning
column header	green	the exposures are filtered on this value
value	green	this value has been modified and is stored in the table
	red	this value fails validation
	light gray	the setting is not applicable for this type of exposure
	dark gray	the type of the exposure has been changed and this setting has become not applicable

Cell	Color	Meaning
	orange	these cells are selected and a new setting can be applied



*Note:* Settings for exposures with multiple subexposures cannot be modified by selecting multiple rows. Select the rows one by one and modify the settings in the settings pane.

### **Export modality settings**

Click **Export modality settings** to create an XML file containing all data in the grid.

This file is intended as an offline reference. Editing or importing data using the XML file is not possible.


## Partial Loading of an Exam Tree

It is possible to load an exam tree from a full export file via the File menu: 'Partial load from file'. This allows exam tree replication between NX systems that share common settings.

### Related Links


[Loading a Partial Configuration from File](#) on page 26



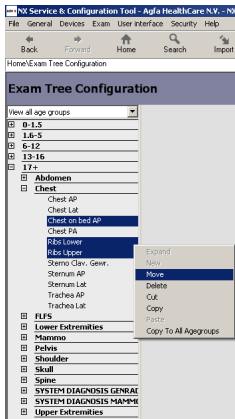

**Figure 102: NX Service and Configuration Tool - Exam Tree - Moving Exposure Types**


Moving one exposure type can also be done by changing its Exam group:

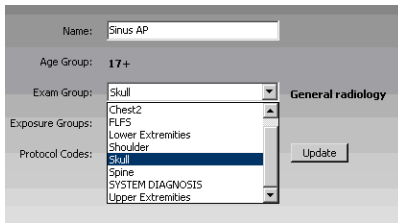

**Figure 103: NX Service and Configuration Tool- Moving Exposure Types.**

## Copying Exposure Types

Select one or more exposure types, or select an exam and copy the exposure types using the context menu 'copy' function (or 'copy exposures'). Multiple exposure types can be selected at once using the CTRL key.

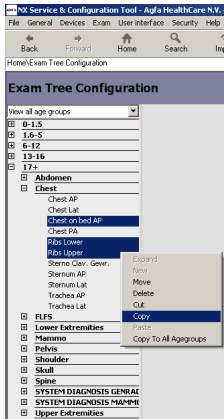

**Figure 104: NX Service and Configuration Tool - Exam Tree - Copying Exposure Types**

Select the target exam group and paste the copied exposure types using the context menu 'paste' function.

The context menu function 'copy to all age groups' can be used to copy one or more exposure types and automatically paste them in the corresponding exam groups of all other age groups.



*Note: If exposure types are copied from one age group to another, Musica1 processing parameters are set to the default of the target age group. The exam tree of a Musica 2 or Musica 3 system also contains Musica 1 processing parameters, as fallback in case the Musica 2 or Musica 3 license is not available anymore.*



*Note: If exposure types that are configured with the Musica 2 or Musica 3 Neo-Natal package are copied to another age group, the copied exposure types will be configured with the Musica 2 or Musica 3 General Radiology package.*



*Note: Modality Settings are not copied but reset to default values.*

## Configuring Examination Groups

Name:

Version:

Application:

Protocol Codes:

Show exam in UI


**Figure 105: NX Service and Configuration Tool - Configuring Examination Groups**

Name	Name (can be edited, will be changed in all age groups)
Version	Shows the version number. Typically only useful for System Diagnostics exam groups. Clicking on it shows the release history.
Application	Indicates the application. Existing applications are: genrad, mammo, dental, uro-tomo, radiotherapy.  Only genrad and mammo exam groups can be created. The others can only be obtained by importing them from older QS systems.  Only genrad and mammo can be used with Musica 2 or Musica 3.
Protocol codes	The protocol code(s) that will cause this exam to be selected in NX when received from RIS.
Show exposure in UI	Whether this exam should be shown in the Add Image pane of NX.  

**Figure 106: NX - Show exam in UI**

A maximum of 21 exams groups can be shown in the Add Image pane. Their position can be configured in the

UI configuration – Compose Exam. Refer to “Compose Exam” .

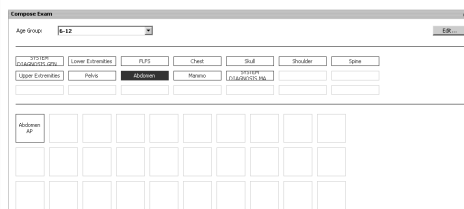

**Figure 107: NX Service and Configuration Tool - Compose Examination**

New button	To create a new exam group. This new exam group will be created for all Age groups.
Delete button	To delete current exam group.
Add exposure button	To create a new exposure (can be put in any exam group, not necessarily current one)
Update button	Allows assigning unlinked protocol codes to this exam group. Another way to do this is via the Edit Protocol Codes page or the Link Protocol Codes page.

### Related Links

[Compose Exam](#) on page 237

## Configuring Exposure Types

---

Each Exposure Type has its private set of processing parameters.

### Musica

Dependent on the Musica2 license, the NX configuration viewer will only show either the Musica 1, Musica 2 or Musica 3 processing parameters.



*Note: Quality assurance images ('System diagnostics') are always processed with Musica 1.*

### X-ray Exposure settings

A set of parameters, used to send to the X-Ray Generator to generate the exposure or (in the case of multiple exposures on 1 cassette) to generate a partial exposure. For a partial exposure, up to 4 settings can be attached to an Exposure type. E.g. for the "Spine cervical LAT + AP" exposure, two exposures have to be made on 1 cassette.

### Topics:


- [General Settings](#)
- [Exposure Settings](#)
- [Processing and Routing](#)
- [Modality Settings](#)

## General Settings


### Topics:

- [General Settings](#)
- [General Settings for FLFS Exposure](#)

## General Settings

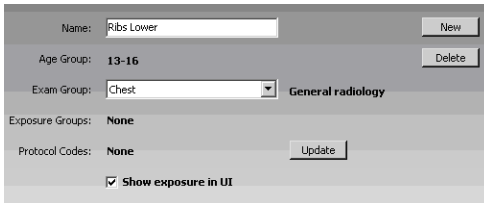


**Figure 108: NX Service and Configuration Tool - Configuring Exposure Types - General Settings**

Name	Name (can be edited)
Age group	The Age group this exposure belongs to.
Exam group	Can be used to move current exposure to the newly selected exam group.
Exposure groups	The exposure groups that use this exposure, see “Exposure Groups”
Protocol codes	The protocol code(s) that will cause this exposure to be selected in NX when received from RIS.
Show exposure in UI	Whether this exposure should be shown in the Add Image pane of NX. 

**Figure 109: NX - Show exposures in UI**

A maximum of 30 exposures per exam group (\*) can be shown in the Add Image pane. Their position can be configured in the UI configuration – Compose Exam. Refer to “Compose Exam” .

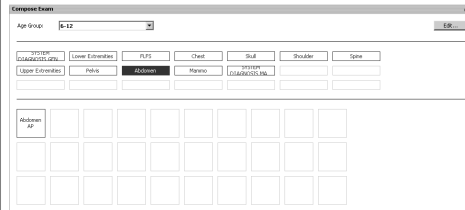

**Figure 110: NX Service and Configuration Tool - Compose examination**


(\*) this includes exposure groups

New button	To create a new exposure (can be put in any exam group, not necessarily current one)
Delete button	To delete current exposure.
Update button	Allows assigning unlinked protocol codes to this exposure.  Another way to do this is via the Edit Protocol Codes page or the Link Protocol Codes page.

**Related Links**

- [Exposure Groups](#) on page 185
- [Compose Exam](#) on page 237

**General Settings for FLFS Exposure**

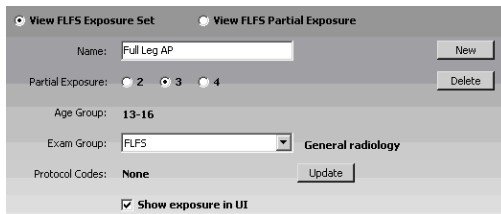

**Figure 111: NX Service and Configuration Tool - General Exposure settings for FLFS Exposure**

View FLFS Exposure set	Shows the exposure settings below for the stitched image. The stitched image is the resulting image after having stitched the separate (partial) images.
View FLFS partial exposure	Shows the exposure settings for the partial (separate) images. The settings apply for all partial images in this set.
Partial exposure	Defines the number of partial images this set consists of.



*Note: For DR FLFS further settings are required.*


### Related Links

[Additional Controls for FLFS examinations](#) on page 177


## Exposure Settings



*Note: The user must be aware that incorrect image orientation may occur due to a wrong value for patient orientation attribute, or selecting the wrong examination type.*

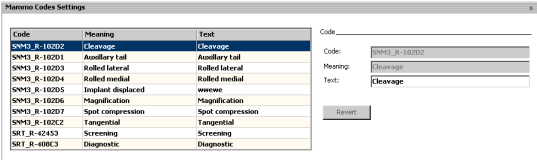Body part	Select a (DICOM) body part.
Auto flip lateral images	<p>Unchecked: lateral images are not flipped.</p> <p>Checked: lateral images are flipped (some hospitals want laterals to face the opposite direction).</p>
Auto rotate 180 degree	<p>Unchecked: default image orientation.</p> <p>Checked: the image is rotated 180 degrees compared to the default image orientation.</p> <p>Only available for DR images.</p> <p>This field is reset when changing modality position.</p>
View position	View position
Anatomic region	The Anatomic Region can be configured with the values from CID 4009 (see DICOM PS 3.16). It is a more precise way to specify the body part, and is used in DX images.
View code	<p>Defines the exposure technique.</p> <p>The view code should be consistent with the view position.</p>
View modifier code	<p>(mammo only)</p> <p>Defines the mammo exposure technique.</p> <p>These values can be ‘translated’ in General Configuration – Mammo codes setting:</p> 

**Figure 112: NX Service and Configuration Tool - View Modifier Code**

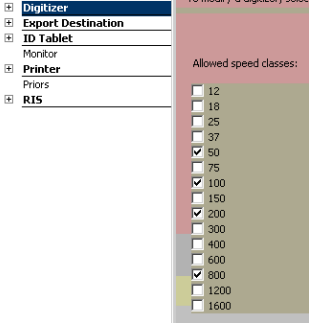Automatically update image laterality when adding marker	When this option is enabled, the image laterality will change from "both" to "left" or "right", as soon as you place a left or right marker respectively. If the image laterality is not "both", it will stay unaffected.
Image laterality	Image laterality.
Implant present	Mammo only.
Cassette orientation	Cassette orientation.
Erasure dose	The dose used to erase the cassette (100mR - 300mR - 750 mR).  More exposed cassettes (direct radiation areas) may require a higher exposure dose (also depending on used body part).
Speed class	Determines the sensitivity used by the Digitizer when scanning a cassette.  This can manually be overruled at run time in NX in the Edit image detail pane.   <p><b>Figure 113: NX Service and Configuration Tool - Speed Class configuration</b></p>
Target Exposure Index	This value is used as reference for Dose Monitoring Statistics on Exposure Index systems. The value is a decimal number with one digit after the decimal point.
Positioning aid	Use the button to select an image file that will be displayed in the image preview pane as a guidance for preparing the exposure.

	If multiple images are available, select an image from the dropdown.
Recommended settings	Type text that will be displayed in the image preview pane as a guidance for preparing the exposure.

**Related Links**

[Configuring Digitizers System Wide](#) on page 75

[Configuring General](#) on page 64

## Processing and Routing

### Topics:

- [Image Processing](#)
- [Automation](#)
- [Printer Settings](#)

### Image Processing

The contents of this pane changes depending on the available Musica (base) license (Musica 1 or 2).

It is beyond the scope of this manual to explain all these settings in detail.

- “Musica 1” .
- “Musica 2” .

### Topics:

- [Musica 1](#)
- [Musica 2 and Musica 3](#)

#### Musica 1

The screenshot shows the 'Image Processing' dialog box for Musica 1. It features a grid of controls:
 

- Collimation:** A dropdown menu set to 'Auto'.
- MUSI Contrast:** A text input field with the value '4'.
- Noise reduction:** A text input field with the value '0'.
- Extended window (left):** A text input field with the value '-0.4'.
- Sensiometric curve:** A dropdown menu set to 'E25'.
- Contrast Nr of Levels:** A dropdown menu set to '3'.
- Focus:** A text input field with the value '0.5'.
- Display collimation border:** A checked checkbox.
- Edge Contrast:** A text input field with the value '0'.
- latitude Reduction:** A text input field with the value '0'.
- Extended window (right):** A text input field with the value '0.3'.
- Threshold value:** A text input field with the value '0.2'.
- Find algorithm:** A dropdown menu set to 'C'.
- WinLatitudeRange:** A label for the range settings below.
- Minimum Value:** A text input field with the value '0.2'.
- Maximum Value:** A text input field with the value '2.5'.
- Copy settings:** A button located at the bottom right of the dialog.


**Figure 114: NX Service and Configuration Tool - Musica 1 dialog box.**

Copy settings button	Allows copying the settings from another exposure to this one.
----------------------	--



*Note: If the default musica processing settings are modified in the NX application using the "Save as default" button in the "Modify MUSICA Settings" dialog, it is advised to make a back-up of these settings, by loading the active configuration in the Service and Configuration Tool and saving it to an external file.*

## Musica 2 and Musica 3

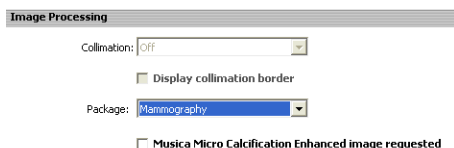

**Figure 115: NX Service and Configuration Tool - Musica 2 and Musica 3 dialog box.**

Collimation	<p>The configuration for auto collimation (which will try to detect diagnostic areas in the image).</p> <p>Not editable in case of mammo exams (always disabled for mammo).</p> <p>Rows\columns:</p> <p>In case of several images on one cassette ('sub exposures'), the rows and columns selection can help the collimation detection algorithm (*). But with current CPU power, this setting can as well be left at 'Auto'.</p>
Display collimation border	<p>During preprocessing of the image, auto-collimation will try to detect diagnostic areas in the image. If this flag is enabled (and the black border license is present), then also a black border is drawn on the non diagnostic areas.</p> <p>The density of the black border can be configured in General Configuration – Workflow management - Image presentation.</p> <p>Available for Musica 1, Musica 2 and Musica 3 but not for mammo.</p>
Package	<p>The Musica 2 or Musica 3 package to be used (list depends on installed license).</p> <p>For some packages (eg. Chest, abdomen, skeleton) both a pediatric and an adult version are present. The NX Service and Configuration Tool doesn't show both packages. It shows only one, the underlying package will be taken by the software depending on the age (&gt; 12years = adult)</p>

	When you get an indication of 'missing license' this means that you do not have (one of) the 'premium' licenses.
Musica Micro Calcification Enhancement image requested	For mammography images identified for an exposure type requesting Musica Micro Calcification Enhancement (MCE), an extra copy of the image is sent to a dedicated archive destination. The extra copy is processed using the MCE image processing.
Enable CATH processing	The CATH button can be made available in the NX Editing environment. The 'CATH' option allows the user to create a copy of the image with a dedicated processing applied to enhance visibility of catheters.  The availability of this option is restricted to diagnostic genrad exposure types.

When configuring the examination tree, verification warning 268 may appear, showing the following text: "There are no exposure types using the specialized Musica 2 or Musica 3 packages".

There exist 6 premium packages:

- chest adults.
- abdomen adults.
- skeleton adults.
- chest pediatrics.
- abdomen pediatrics.
- skeleton pediatrics.

They belong to the NX Musica 2 or Musica 3 PLATINUM license.

As long as there is not at least 1 exposure configured for each existing premium package, Verification warning 268 will appear.

So, for the warning to disappear you need to configure an exposure type for each of the 6 packages.

- For the first 3 you need to take an exposure in age groups 17+ or 13-16 (older than 12 years is considered 'adult')
- For the last 3 you need to take an exposure in of one of the other age groups





*Note: System diagnostics exposures only use Musica 1 and are not editable.*


**Related Links**

- [Image Presentation](#) on page 58
- [Managing Licenses](#) on page 143
- [Action Buttons](#) on page 242

**Automation**
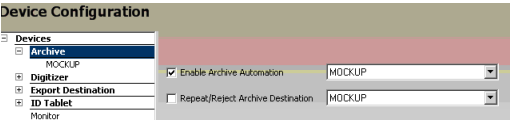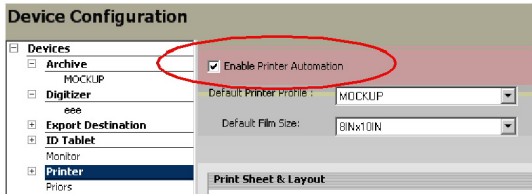
<p>Automatically archive image</p>	<p>When enabled, image will automatically be sent to the general automation destination as configured in the Archive setup.</p>  <p><b>Figure 116: NX Service and Configuration Tool - Automatic Archiving configuration</b></p> <p>When the general archive automation is disabled, then this functionality is also automatically disabled here.</p>
<p>Automatically print image</p>	<p>When enabled, image will automatically be sent to the general automation destination as configured in the Printer setup.</p>  <p><b>Figure 117: NX Service and Configuration Tool - Automatic printing configuration</b></p> <p>when the general print automation is disabled, then this functionality is also automatically disabled here.</p>
<p>additional destinations</p>	<p>when configured, the image will (additionally) be sent to these destinations. (this setting does not depend on 'automatically archive image')</p>

when the general archive automation is disabled, then this functionality is also automatically disabled here.



**Figure 118: nx service and configuration tool - additional destinations**

'Enable archive automation' is enabled.


	'Automatically archive image'	'Additional destinations'
Exposure 1:	Disabled	Archive A
Exposure 2:	Disabled	Archive B



*Note: Following setup allows to send exposure 1 to archive A and exposure 2 to archive B.*

## Printer Settings

FilmSize	<p>Can be put on DEFAULT or on a specific film size.</p> <p>DEFAULT: means depending on the cassette size the film size is taken and from this the printer is chosen. All this is configured in the printer setup screen. 'DEFAULT' is not allowed for FLFS Stitched image since a FLFS Stitched image does not come from one cassette.</p> <p>On a specific film size: then the corresponding printer is taken from the setup in the printer setup screen</p> <p>Printer setup screen:</p>
----------	---

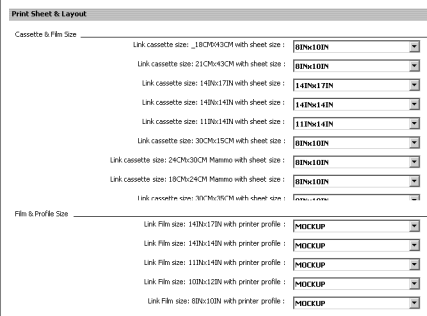	 <p><b>Figure 119: NX Service and Configuration Tool Printer Settings - Film Size</b></p>
Printer & film size	The specific printer & film size will be used.
Textbox position	Only valid for a 1/1 layout.
Scale mode	True size or best fit.
Film orientation	Only applies to exposures on a DR Detector. The automatic setting links the film orientation to the orientation of the exposed area. The film orientation can also be forced to a specific setting.

## Related Links

[Modality Exposure Settings](#) on page 180

## Modality Settings

The NX Workstation can be connected to:

- the X-Ray System Generator to send and receive X-Ray exposure setting and
- a DR Detectors to exchange image data

These settings are only available when:

- XRDI software is installed next to NX on the PC
- The correct licenses for DX-Si ('IDIS1 Connection') and optionally for DR Workflow are installed.
- Musica mammo license is not enabled
- An X-Ray device is configured. This is a genrad type of modality (e.g. GEN IT generator or Quantum Techvision), optionally including DR functionality.

In the Modality Settings pane, you can configure the attributes of the connected modality for each exposure type in the examination tree. The set of configurable modality settings depends on the modality type.

When an exposure type is selected during identification the configured modality settings are sent out as presets to the X-Ray device console.

### Related Links

[Configuring the X-Ray Device](#) on page 127

### Topics:

- [Modalities with DR functionality](#)
- [Modalities without DR functionality](#)

### Modalities with DR functionality

#### Topics:

- [Modality Exposure Settings](#)
- [Modality Position and Receptor Type Settings](#)
- [Additional Controls](#)
- [Additional Controls for FLFS examinations](#)
- [Exposure Views \(subexposures\)](#)
- [Modality Settings Examples](#)

## Modality Exposure Settings

The screenshot shows the 'Modality Exposure Settings' window. It features several control elements:

- kVp:** A dropdown menu set to '43' with up and down arrow buttons.
- mAs:** An empty input field with up and down arrow buttons.
- max ms:** A dropdown menu set to '550' with up and down arrow buttons.
- AEC Sensitivity:** Three radio button options: High sensitivity [H] (selected), Universal [U], and Detail [D].
- AEC Chambers:** Three radio button options: [None], Universal [U] (selected), and Detail [D].
- AEC Density:** A dropdown menu set to '0' with up and down arrow buttons.
- Focus:** Two radio button options: Small focus and Large focus (selected).
- Grid:** Two radio button options: Grid (selected) and None.
- PreFilter:** A dropdown menu set to 'None'.
- Exposed Area (mm):** Two dropdown menus: 'Longitudinal/Height' set to '430' and 'Transverse/Width' set to '430', both with up and down arrow buttons and a '...' button.

**Figure 120: NX Service and Configuration Tool - Modality Settings - Exposure Type section**

AEC Detector Sensitivity	The selection of detector sensitivity defines the cut-off dose of the AEC chambers for the exposure. The settings for detector sensitivity (High sensitivity [H], Universal [U] and Detail[D]) rely on calibration during installation of the X-Ray System. The selection of density defines a correction expressed in EP (Exposure Points) that can be used for patient transparency compensation. The default setting for the exposure should be 0.
Exposed Area	Only applicable for exposures on a DR Detector. The exposed area defines the area on the detector to which exposure is limited by means of collimation. Using the drop-down button, matching cassette sizes can be selected.
AEC Density	The selection of density defines a correction expressed in EP (Exposure Points) that can be used for patient transparency compensation. The Default setting for the exposure should be 0.



*Note: When setting the kV and mAs values, the user must be aware that the validation of the entered values does not take in account the power of the generator (GEN IT 80 is assumed), the selection of the focus (large focus is assumed) and the power value (100% is assumed). This means that when both the maximum for kV and mAs are configured as preset, and the generator does not meet the entered maxima, the generator will be set on lower values by generator protection.*

## Modality Position and Receptor Type Settings

- For systems with DR functionality:




**Figure 121: NX Service and Configuration Tool - Modality Settings - Modality Position**

Modality Position	Refer to the NX User Manual for the meaning of the modality position icons (Section Using Examinations).  The available modality positions depend on the installed and configured X-Ray Device.
Nickname	A portable DR Detector must be identified by its nickname.

### Additional Controls

For modalities that provide extra controls, e.g. positioning of the modality, additional panes are displayed to store the default settings for the exposure.

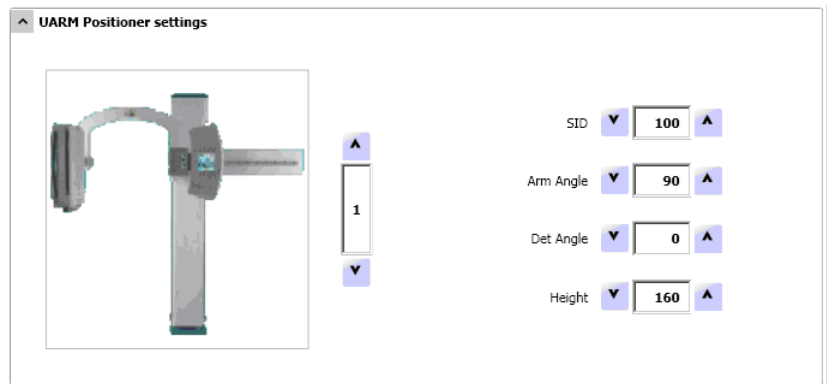


**Figure 122: Settings for positioning of a U-arm modality.**

### Additional Controls for FLFS examinations

For modalities that support the automatic FLFS workflow, additional controls are available in the modality positioner settings pane.

To configure the automatic FLFS workflow

1. Go to the modality Positioner Settings pane in the Exposure screen.

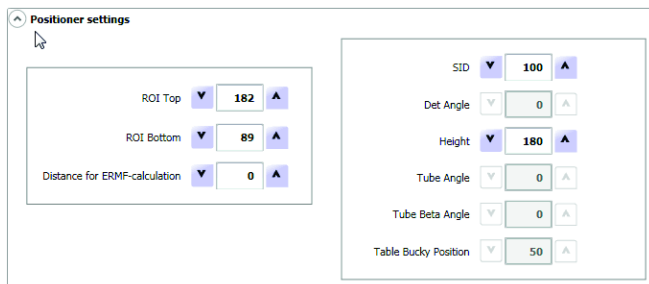

**Figure 123: Positioner Settings**

2. If the FLFS examination uses a portable DR Detector, select its nickname in the drop-down list.
3. Define default values for
  - the distance between the stitching grid of the DX Full Leg Full Spine stand and the patient. This value is used to apply ERMF-calibration on the stitched image.
  - the top of the ROI
  - the bottom of the ROI
4. For the top partial image, define a default position:
  - the height of the DR Detector (applies only when using the DX Full Leg Full Spine Stand)
  - the SID

The modality will move into this position to prepare the FLFS examinations.

5. For each partial image, define the Modality Exposure Settings by adding an exposure view for each partial image. If more partial images are needed than defined in the examination, the settings for the last partial image will be repeated.
6. Go to the Image Processing pane in the Exposure screen and select the availability and position of the Stitch Quality Annotation. The Stitch Quality Annotation is a text annotation that can automatically be added to the image, containing information about the stitching process.

### Exposure Views (subexposures)

Multiple views can be used when examinations require more than one exposure on a cassette.

To add a subexposure

1. Click the '+'-button at the bottom left of the Modality Settings pane.
2. Apply the settings for this subexposure.

Navigate from one subexposure to another using the navigation buttons at the top left of the Modality Settings pane.



Note: Multiple views are not available for exposures on a DR Detector.



Figure 124: NX Service and Configuration Tool - Modality Settings - Exposure with two subexposures defined

### Modality Settings Examples

#### Topics:

- [Defining a DR Table Exposure](#)

#### *Defining a DR Table Exposure*

You can choose to define a DR Table Exposure with Automatic Exposure Control (AEC) or without AEC.

#### Topics:

- [To define a DR Table Exposure with AEC:](#)
- [To define a DR Table Exposure without AEC:](#)

To define a DR Table Exposure with AEC:

1. Click the icon for fixed DR Detector in the table.



Figure 125: NX Service and Configuration Tool - icon for fixed DR Detector in the table

2. Select the AEC chambers to be used.

By default, the middle one will be selected. All combinations are possible.

As a result of the choice for AEC:

- The examination technique will be kV.
- The Focus will be enabled.
- Detector sensitivity will be enabled.
- Density parameter will be enabled.
- kV field will be enabled under Exposure Views.
- mAs field will be disabled under Exposure Views.

### 3. Configure the enabled parameters.

To define a DR Table Exposure without AEC:

#### 1. Click the icon for free exposure using the Portable DR Detector.

**Figure 126: NX Service and Configuration Tool - icon for free exposure using the Portable DR Detector.**

#### 2. Deselect the middle AEC chamber (which is selected by default). No AEC chambers should be selected.

As a result of the choice for disabling AEC:

- The examination technique will be kV, mAs.
- The Focus will be enabled.
- Detector sensitivity will be disabled.
- Density parameter will be disabled.
- kV field will be enabled under Exposure Views.
- mAs field will be enabled under Exposure Views.

#### 3. Configure the enabled parameters.

## Modalities without DR functionality

### Topics:

- [Modality Exposure Settings](#)
- [Modality Position and Receptor Type Settings](#)
- [Exposure Views](#)
- [Modality Settings Examples](#)

### Modality Exposure Settings

**Figure 127: NX Service and Configuration Tool - Modality Settings - Exposure Type section**

AEC Detector Sensitivity	The selection of detector sensitivity defines the cut-off dose of the AECchambers for the exposure. The settings for detector sensitivity (High sensitivity [H], Universal
--------------------------	--

	[U] and Detail[D]) rely on calibration during installation of the X-Ray System. The selection of density defines a correction expressed in EP (Exposure Points) that can be used for patient transparency compensation. The default setting for the exposure should be 0.
Exposed Area	Only applicable for exposures on a DR Detector. The exposed area defines the area on the detector to which exposure is limited by means of collimation. Using the drop-down button, matching cassette sizes can be selected.
AEC Density	The selection of density defines a correction expressed in EP (Exposure Points) that can be used for patient transparency compensation. The Default setting for the exposure should be 0.

### Modality Position and Receptor Type Settings

- For systems without DR functionality:



**Figure 128: NX Service and Configuration Tool - Modality Position**


Modality Position	Defines if the exposure is a table exposure, a wall exposure or a free exposure.  The Modality Position information is located in the Exposure Type section of the Modality Settings pane.
-------------------	--

### Exposure Views

With the Add View button you set the actual exposure parameters and you can continue with a new definition. Multiple views can be used when examinations require more than one exposure on a cassette. The Add View button is located bottom right in the Exposure Type section of the Modality Settings pane.



*Note: Multiple views are not available for exposures on a DR Detector.*

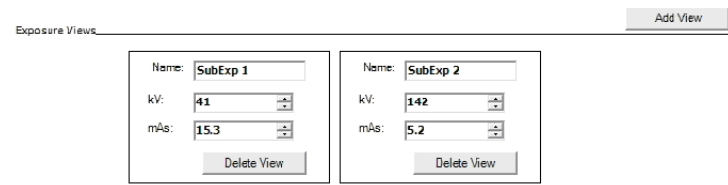

**Figure 129: NX Service and Configuration Tool - Modality Settings - Exposure Views section**



*Note: When setting the kV and mAs values, the user must be aware that the validation of the entered values does not take in account the power of the generator (GEN IT 80 is assumed), the selection of the focus (large focus is assumed) and the power value (100% is assumed). This means that when both the maximum for kV and mAs are configured as preset, and the generator does not meet the entered maxima, the generator will be set on lower values by generator protection.*

### Modality Settings Examples

#### Topics:

- [Defining a CR Wall Exposure](#)

#### *Defining a CR Wall Exposure*

You can choose to define a CR Wall Exposure with Automatic Exposure Control (AEC) or without AEC.

#### Topics:

- [To define a CR Wall Exposure with AEC:](#)
- [To define a CR Wall Exposure without AEC:](#)

To define a CR Wall Exposure with AEC:

1. Select the CR Wall Exposure radio button.



**Figure 130: NX Service and Configuration Tool - CR Wall Exposure radio button**

2. Select the AEC chambers to be used.

By default, the middle one will be selected. All combinations are possible.

As a result of the choice for AEC:

- The examination technique will be kV.
- The Focus will be enabled.

- Detector sensitivity will be enabled.
  - Density parameter will be enabled.
  - kV field will be enabled under Exposure Views.
  - mAs field will be disabled under Exposure Views.
3. Configure the enabled parameters. The table below shows the possible values:

Parameter	Possible value
Focus setting	Small - Large
Detector Sensitivity Setting	D _ U _ H
Density	-3 / +3
kV	40 - 150 kV

To define a CR Wall Exposure without AEC:

1. Select the Free Exposure radio button.



**Figure 131: NX Service and Configuration Tool - Free Exposure radio button**

2. Deselect the middle AEC chamber (which is selected by default). No AEC chambers should be selected.

As a result of the choice for disabling AEC:

- The examination technique will be kV, mAs.
  - The Focus will be enabled.
  - Detector sensitivity will be disabled.
  - Density parameter will be disabled.
  - kV field will be enabled under Exposure Views.
  - mAs field will be enabled under Exposure Views.
3. Configure the enabled parameters. The table below shows the possible values:

Parameter	Possible value
Focus setting	Small - Large
kV	40 - 150 kV
mAs	0,5 to 800 mAs

## Configuring Exposure Groups

---

An Exposure group is a collection of Exposure types. It can be linked to a protocol code. By default, all Exposure types will print on separate print sheets. Special print templates can be assigned to automatically print selected Exposure Types on the same print sheet.

### Topics:

- [Exposure Groups](#)
- [Creating Exposure Groups](#)
- [Editing Exposure Groups](#)


## Exposure Groups

Beside the three levels that make up an NX exam tree (age groups, exam groups, exposure types), there exist also the concept of 'exposures groups'.

An exposure group is a collection of (one or more) exposure types. It can contain exposure types of different age groups. When the exposure group is used in an examination, only the exposure types of the age group the patient belongs to are added to the examination. Also, the order of the exposure types can be specified per age group. This order will be used for displaying the exposure types in the image overview pane.

An exposure group can be configured to be selectable in the NX user interface to allow manual selection of the exposure group when starting an examination.

An exposure group is indicated in NX as follows:




**Figure 132: NX - Exposure Groups presentation**

Example: create exposure group X with contents:

- 1. Chest Lat (17+, Chest)**
- 2. Ribs Upper (17+, Chest)**
- 3. Chest PA (13-16, Chest)**

**Figure 133: NX Service and Configuration Tool - contents of exposure group**

When in NX an exam is created, the 17+ selection screen will look as follows:

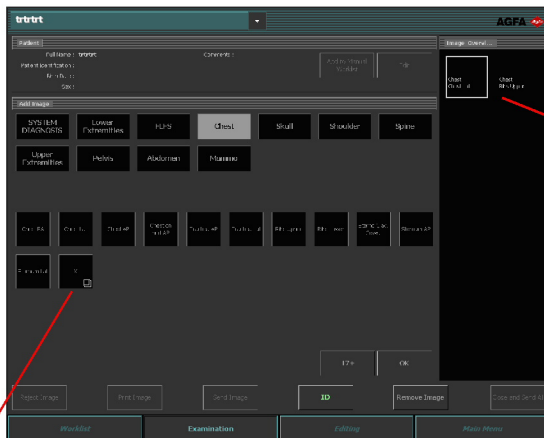


Only the 17+ exposures of this exposure group are shown

Exposure group X

Figure 134: NX Exposure group example in NX

For 13-16:

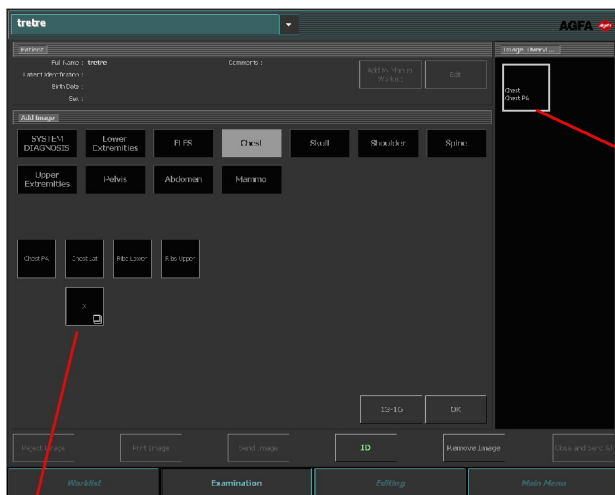

Only the 13-16 exposures of this exposure group are shown

Exposure group X

Figure 135: NX Exposure group example for 13 - 16

An exposure group can be linked to a protocol code (to allow automatic selection of the exposures of the exposure group when the protocol code is received from the RIS). This is the same as for an exposure or an exam.

For protocol codes, please refer to “Automatic Selection of Exposure, Exam or Exposure group” for an overview on protocol codes.

Finally, for each age group, the exposure types in the exposure group can be linked to print profiles allowing automatic printing of multiple exposure types on a sheet in a preconfigured way.






*Note: If it doesn't contain any Exposure Types for the Age group of that patient, the Exposure Group will not be visible during normal NX operation.*

### **Related Links**

[Automatic Selection of Exposure, Exam or Exposure group](#) on page 123

## Creating Exposure Groups

Exposure groups can be created in different ways:
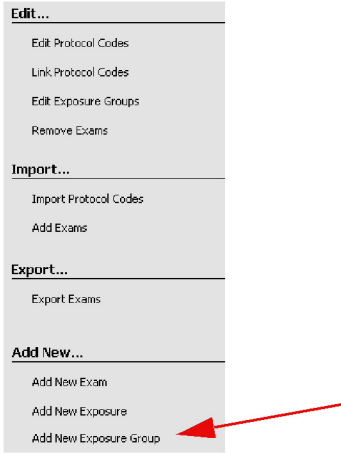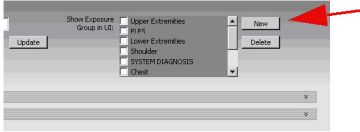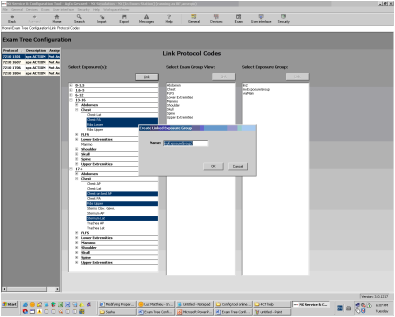
<p>... In the main exam tree pane: Add new exposure group</p>	 <p><b>Figure 136: NX Service and Configuration Tool - creating exposure groups</b></p>
<p>... in the edit exposure groups pane:</p>	 <p><b>Figure 137: nx service and configuration tool - creating exposure groups</b></p>
<p>... in the link protocol codes pane:</p>	 <p><b>Figure 138: nx service and configuration tool - creating exposure groups</b></p> <p>Details see: “Linking Protocol Codes”.</p>

## Related Links

[Configuring Exposure Groups](#) on page 184


[Linking Protocol Codes](#) on page 195

## Editing Exposure Groups

In this pane, exposure groups can be created, changed or deleted.

Exposure groups can also be created in “Linking Protocol Codes”

Name	Change its name
Protocol code	The protocol code(s) that will cause this exposure group to be selected in NX when received from RIS.
Show exposure group in UI	Under which exam group to show this exposure group in NX, see further
Enable Automated DR Full Screen Sequence	When enabled: After acquiring an image, the image is displayed in full screen mode and the next thumbnail is selected automatically.
New button	To create a new exposure group
Delete button	To delete current exposure group
Update button	Allows assigning unlinked protocol codes to this exposure group.  Another way to do this is via the Edit Protocol Codes page or the Link Protocol Codes page.

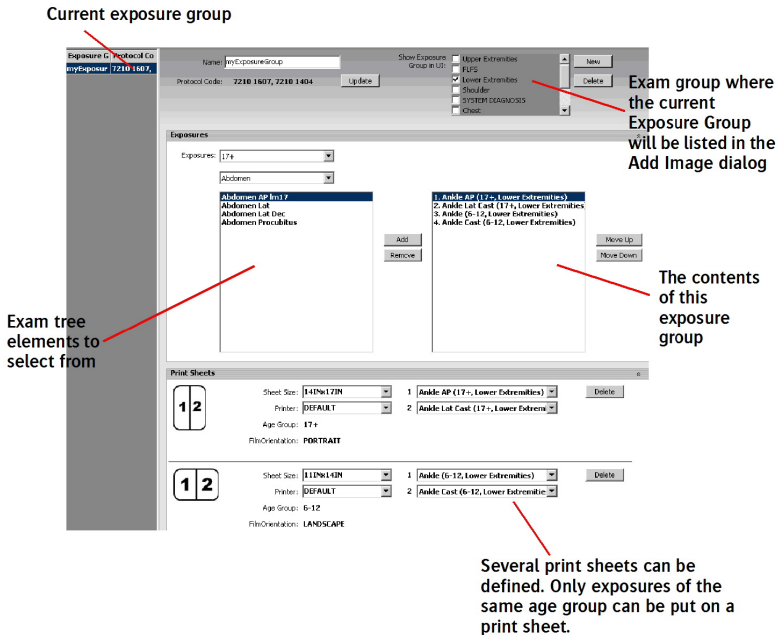

**Figure 139: NX Service and Configuration Tool - Overview editing exposure groups.**

**Related Links**

[Linking Protocol Codes](#) on page 195

**Topics:**

- [Show Exposure group in UI](#)
- [Adding a New Print Sheet Dialog Box](#)

**Show Exposure group in UI**

The configuration screen allows to select the Exam Group where the current Exposure Group will be listed in the Add Image dialog.

The software will automatically pick the next free cell in the Exam Group to display the Exposure Group..

If an Exam Group has no free cells, it is not listed (an Exam Group can contain only 30 elements).

If the Exposure Group contains exposures of different Age Groups, the Exam Group must have a common free cell for all Age Groups in order to be listed.

Example:

The following example shows the examination composition of an Exam Group in the two Age Groups that are contained by the Exposure Group. The first common free cell is number five.

**Compose Exam**

Age Group: **6-12**

---

SYSTEM DIAGNOSTIS_GEN	Lower Extremities	FLFS	Chest	Skull	Shoulder	Spine
Upper Extremities	Pelvis	<b>Abdomen</b>	Mammo	SYSTEM DIAGNOSTIS_MA		

---

Abdomen AP				myExposureGroup					

**Figure 140: NX Service and Configuration Tool - Editing Exposure Groups**

**Compose Exam**

Age Group: **17+**

---

SYSTEM DIAGNOSTIS_GEN	Lower Extremities	FLFS	Chest	Skull	Shoulder	Spine
Upper Extremities	Pelvis	<b>Abdomen</b>	Mammo	SYSTEM DIAGNOSTIS_MA		

---

Abdomen AP	Abdomen Lat	Abdomen Procrubitus	Abdomen Lat Dec	myExposureGroup					

**Figure 141: NX Service and Configuration Tool - Editing Exposure Groups**

**Related Links**

[Compose Exam](#) on page 237

## Adding a New Print Sheet Dialog Box

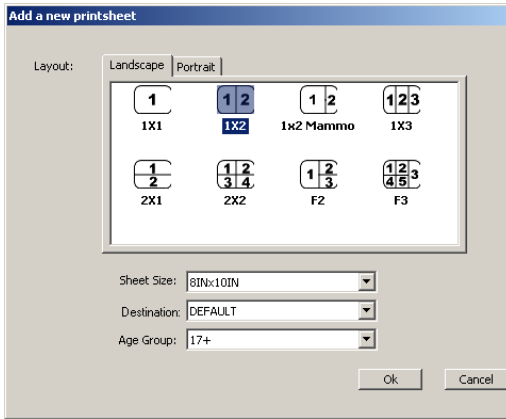


Figure 142: Adding a New Print Sheet dialog box.

When selecting the DEFAULT destination, the printer is defined in the printer setup page under 'Film & profile size' depending on the configured sheet size.

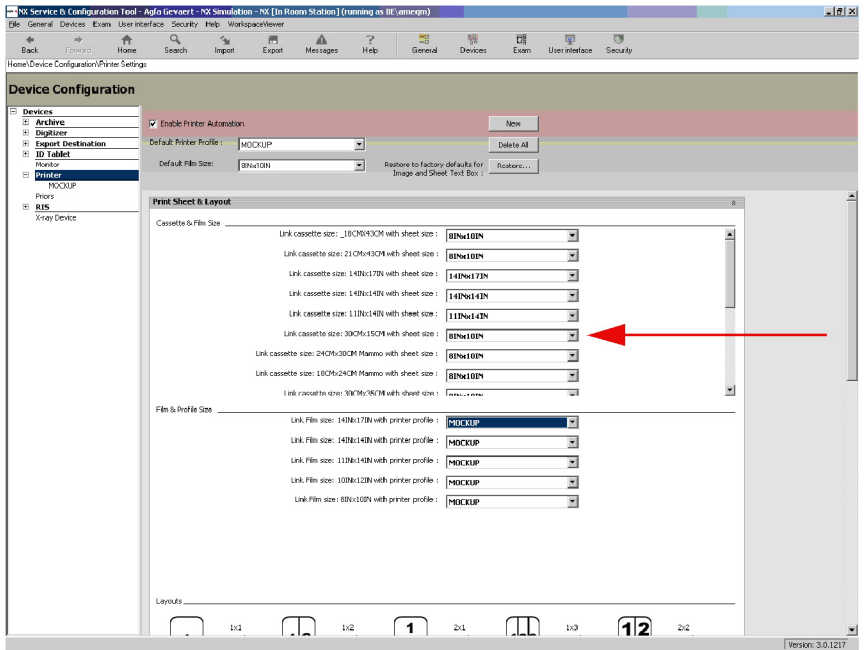


Figure 143: Configuring Printers page - Printer definition.

## Managing Protocol Codes

---

### Topics:

- *Importing Protocol Codes*
- *Linking Protocol Codes*
- *Adding new Protocol Codes*
- *Editing Protocol Codes*
- *Removing Protocol Codes*
- *Unassigning Protocol Codes*
- *Adding Unknown Protocol Codes*
- *Exporting Protocol Codes*

## Importing Protocol Codes

The user can import a list with protocol codes in the NX Service and Configuration Tool. The protocol codes of that list can then be assigned to Exposure types, to Exposure groups or to Examination groups.

To import a list with protocol codes:

1. Click **Import protocol codes** in the main form.


A Windows file selection dialog box appears.

2. Select the file with protocol codes and click **Import**.

### Related Links

[Adding new Protocol Codes](#) on page 198

## Importing
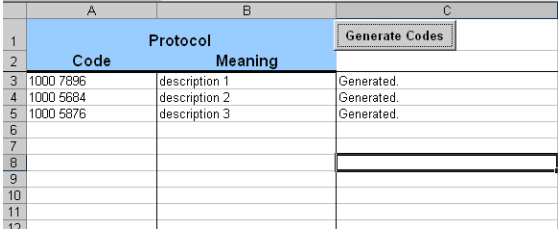
<p>Import protocol codes</p>	<p>Select an xml file with protocol codes.</p> <p>The xml file can be generated with the Protocol code template in Microsoft Excel. (see Start Menu – Agfa- NX – Service – Install Tools – Protocol Code template (Excel2000 only).</p>  <p><b>Figure 144: NX Service and Configuration Tool - Importing Protocol Codes</b></p> <p>The imported protocol codes are added to the list of non-assigned protocol codes. Next step is to link or edit them manually.</p>
<p>Add exams</p>	<p>Select an xml file with previously exported exams (you cannot use a full export file here).</p> <p>Brings up a selection box with the exams available in the xml file from which you can select.</p>

## Linking Protocol Codes

This screen allows you to easily link protocol codes to

- an exposure type
- or an exam group
- or an exposure group

At the left side, only protocol codes are shown that are not yet linked.

To link a protocol code:

1. Select a protocol code and then select an exposure or an exam group or and exposure group.
2. Press the corresponding Link button at the top of the list.


## Related Links

[Automatic Selection of Exposure, Exam or Exposure group](#) on page 123

## Creation of new Exposure Groups

Also, new exposure groups can be created in this pane and immediately linked to protocol codes.

When more than one exposure from the exposure list is selected (use CTRL key), then an exposure creation dialog pops up when pressing the Link button.

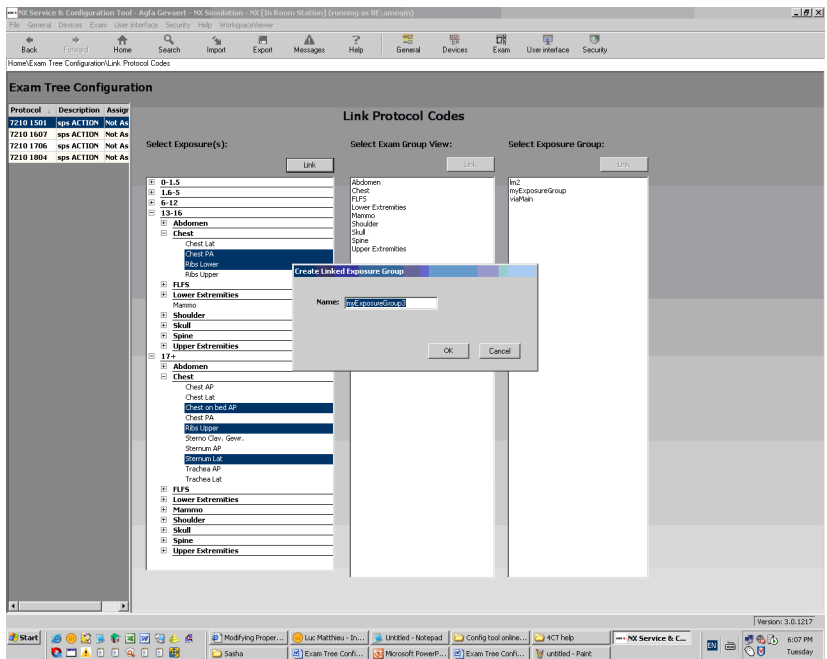

**Figure 145: NX Service and Configuration Tool - Creating Exposure Groups**

Enter a name and press OK to create a new exposure group. Further editing of this exposure group (including visibility in the Add Image pane on NX) can be done in the Edit exposure group name pane.

**Related Links**

[Configuring Exposure Groups](#) on page 184

## Adding new Protocol Codes

Apart from importing a file with protocol codes, the user can also add individual protocol codes to the Protocol Code list.


To add a new protocol code:

1. Click **Edit Protocol Codes** in the Exam Tree Configuration window.

The Edit Protocol Codes main window appears.

2. Press the **New** button in the Edit Protocol Codes main window.

The **Add Protocol Code** dialog box is displayed:

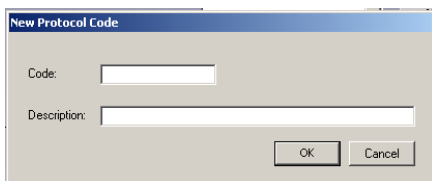

**Figure 146: NX Service and Configuration Tool - Add New Protocol Code dialog box.**

3. Enter the protocol code value and/or description.
4. Press **OK** to confirm your choice, otherwise click **Cancel**.

If you have pressed OK the system adds the protocol code to the list.

### Related Links


[Importing Protocol Codes](#) on page 195

## Editing Protocol Codes

This screen allows you to create, load, edit and delete protocol codes.

At the left side of the screen, all protocol codes known to the system are shown. Unassigned codes are indicated ('Not Assigned').

Linking of unassigned protocol codes can also be done in the linking protocol code screen.

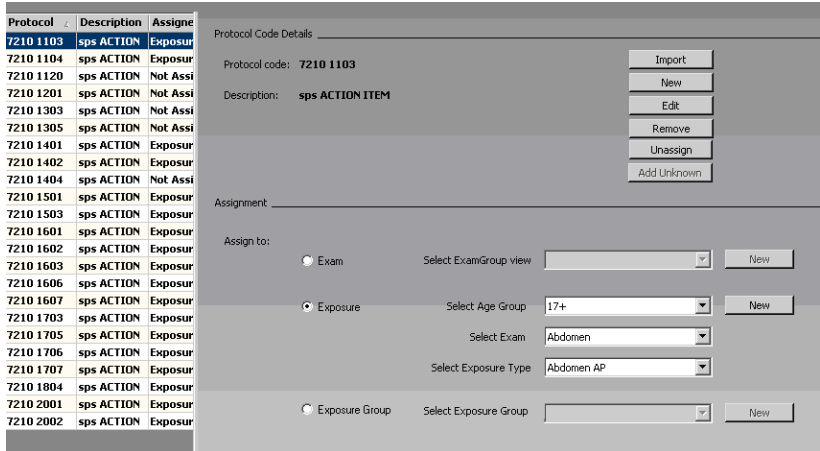

**Figure 147: NX Service and Configuration Tool - Editing Protocol Codes**

<p>Import button</p>	<p>Load protocol codes from an xml file.</p> <p>The xml file can be generated with the Protocol code template in Microsoft Excel. (see Start Menu – Agfa- NX – Service – Install Tools – Protocol Code template (Excel2000 only).</p> <table border="1" data-bbox="367 1068 931 1299"> <thead> <tr> <th></th> <th>A</th> <th>B</th> <th>C</th> </tr> </thead> <tbody> <tr> <td>1</td> <td colspan="2">Protocol</td> <td rowspan="2">Generate Codes</td> </tr> <tr> <td>2</td> <td>Code</td> <td>Meaning</td> </tr> <tr> <td>3</td> <td>1000 7896</td> <td>description 1</td> <td>Generated.</td> </tr> <tr> <td>4</td> <td>1000 5684</td> <td>description 2</td> <td>Generated.</td> </tr> <tr> <td>5</td> <td>1000 5876</td> <td>description 3</td> <td>Generated.</td> </tr> <tr> <td>6</td> <td></td> <td></td> <td></td> </tr> <tr> <td>7</td> <td></td> <td></td> <td></td> </tr> <tr> <td>8</td> <td></td> <td></td> <td></td> </tr> <tr> <td>9</td> <td></td> <td></td> <td></td> </tr> <tr> <td>10</td> <td></td> <td></td> <td></td> </tr> <tr> <td>11</td> <td></td> <td></td> <td></td> </tr> <tr> <td>12</td> <td></td> <td></td> <td></td> </tr> </tbody> </table>		A	B	C	1	Protocol		Generate Codes	2	Code	Meaning	3	1000 7896	description 1	Generated.	4	1000 5684	description 2	Generated.	5	1000 5876	description 3	Generated.	6				7				8				9				10				11				12			
	A	B	C																																																	
1	Protocol		Generate Codes																																																	
2	Code	Meaning																																																		
3	1000 7896	description 1	Generated.																																																	
4	1000 5684	description 2	Generated.																																																	
5	1000 5876	description 3	Generated.																																																	
6																																																				
7																																																				
8																																																				
9																																																				
10																																																				
11																																																				
12																																																				
<p>New button</p>	<p>To enter a new protocol code</p>																																																			

Edit button	To change name and or description of the selected protocol code
Remove button	To delete a protocol code and its links
Unassign button	To undo an assignment of a protocol code to an exposure, exam group or exposure group.
Add unknown button	NX keeps track of protocol codes received from the RIS during previous NX runs which are not assigned to an exposure yet (or exam group or exposure group).  With this button, it is possible to add these to the protocol code list and assign them.

### Related Links

[Automatic Selection of Exposure, Exam or Exposure group](#) on page 123

[Linking Protocol Codes](#) on page 195

## Removing Protocol Codes

The user can remove individual protocol codes from the Protocol Code list.

To remove protocol codes:

1. Click **Edit Protocol Codes** in the Exam Tree Configuration window.


The Edit Protocol Codes main window appears.

2. Select a protocol code from the Protocol Code list pane.

The red box shows the position of the selected protocol code:

3. Press the **Remove** button in the Edit Protocol Codes main window.

The system will display a warning message:

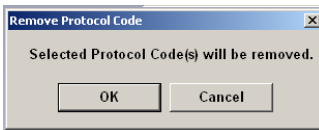

**Figure 149: NX Service and Configuration Tool - Removing Protocol Codes**

4. Press **OK** to confirm your choice, otherwise click **Cancel**.

If you have pressed OK the system will remove the protocol code from the list.

## Unassigning Protocol Codes

It is possible to undo an assignment of a protocol code.

To unassign protocol codes:

1. Click **Edit Protocol Codes** in the Exam Tree Configuration window.

The Edit Protocol Codes main window appears.

2. Perform the following actions:

- Select a protocol code from the Protocol Code list pane.
- Click Unassign.
- In the Confirm dialog, click Yes.

## Adding Unknown Protocol Codes

It is possible that an examination with an unknown protocol code enters NX during the hospital workflow. Images with an unknown protocol code are marked with a question mark in the empty thumbnail.

You can decide to add the unknown protocol codes to the NX Service and Configuration Tool. When this is done, you can link these protocol to exposure types, exposure groups or examination groups.

To add unknown protocol codes:

1. Click **Edit Protocol Codes** in the Exam Tree Configuration window.  
The Edit Protocol Codes main window appears.
2. Click the **Add Unknown** button.

### Related Links

[Linking Protocol Codes](#) on page 195

## Exporting Protocol Codes

Click the link **Export protocol codes** to create an XML file containing the list of protocol codes.

# Configuring the User Interface

---

## Topics:

- *General Settings*
- *Worklist Settings*
- *Examination Settings*
- *Editing Settings*

## General Settings

---

In the NX Service and Configuration Tool General Settings User Interface Settings section, the user can configure the general look and feel settings of NX.

### Topics:

- [\*Person Name Configuration\*](#)
- [\*Image Overview\*](#)
- [\*Current Patient Switch\*](#)
- [\*Configuring External Applications\*](#)

## Person Name Configuration

In the Main pane of the General Settings section, the person name configuration is performed.

### Topics:


- [Person Name Composition](#)
- [Person Name Representation](#)

### Person Name Composition

For the available person names, the person name composition can be defined. A full name is composed of the elements:

- Prefix
- Last Name
- First Name
- Middle Name
- Suffix

The order of the full name elements is configured by selecting the values in the desired order from the drop-down boxes:




**Figure 150: NX Service and Configuration Tool – Person Name Composition**

The configured full name composition will be applicable for all available full name attributes:

- Patient name
- Birth name
- Operator name
- Referring Physician name
- Performing Physician name
- Requesting physician
- Operator name

The configured full name composition will be used within NX on locations where the full name is displayed, e.g.:

- Patient Switch



**Figure 151: NX– Person Name Composition in the Patient Switch**


- Grids as Worklist, Closed Exams List...

Worklist (3) - DICOMXML			
	Patient Name		Accession Number
	David Caruso 1956-12-12...	Male	
	Mr Jones Bart Hugo... 1976-01-01...	PatID12345 Male	
	El AL Chaled... 1911-09-11...	M3070 Female	PD7555

**Figure 152: NX– Person Name Composition in the Worklist**

## Person Name Representation

For the available person names, the person name representation mode can be defined.

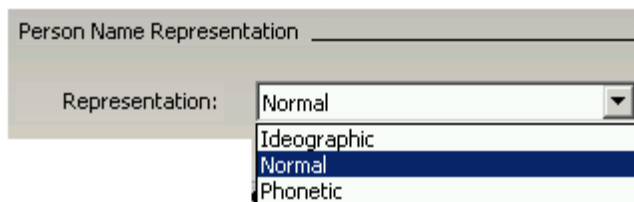

**Figure 153: NX Service and Configuration Tool – Person Name Representation**

From the drop-down box select one of these settings:

- Normal
- Ideographic
- Phonetic

The selected code set for the person name representation is dependent of the DICOM character set configuration in the Workstation Settings.



*Note: The Name Representation on a Central Monitoring System must be the same as on the in-room NX Workstations.*

### Related Links

[Workstation General Settings](#) on page 40

## Image Overview

In the Image Overview pane, the displayed attributes of the exposure and image thumbnails can be configured.



**Figure 154: NX Service and Configuration Tool – Image Overview pane**

The exposure and image thumbnails are displayed throughout the application in the NX image overview pane:



**Figure 155: NX– Image Overview pane**


For the exposure thumbnails up to three attributes can be configured for display. For the image thumbnails up to four attributes can be configured for display.



*Note: It is possible to leave values blank, thereby allowing spatial configuration of the attributes.*

## Current Patient Switch

The “Current Patient Switch” pane allows the configuration of the Examination environment patient switch.

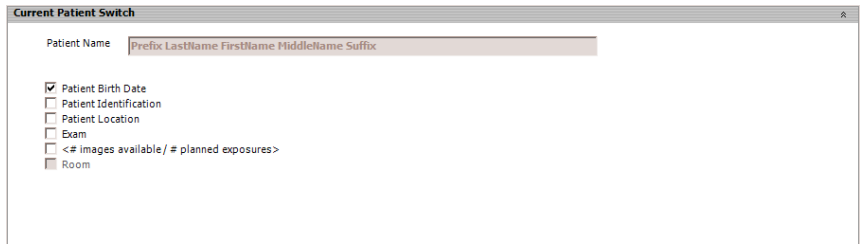


**Figure 156: NX Service and Configuration Tool – Current Patient Switch pane**

The displayed patient name(s) composition is defined within this section of the NX Service and Configuration Tool.

The displayed patient name consists by default of the configured name representation “Person Name Configuration” optionally appended with one of the following options:

- Patient Birth Date

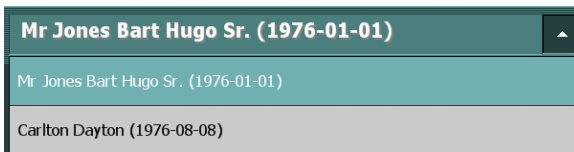

**Figure 157: NX – Examination environment Patient Switch with optionally configured birth date indication**

The patient birth date is displayed in the configured regional settings format of NX.


- Patient Identification

The Patient Identification is displayed.

- Patient Location


The Patient Switch displays where the patient is located in the hospital.

- Exam

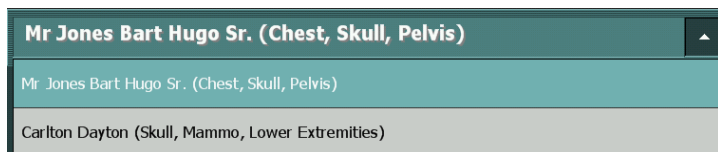

**Figure 158: NX – Examination environment Patient Switch with optionally configured exam indication**

- <# images available/# planned exposures>

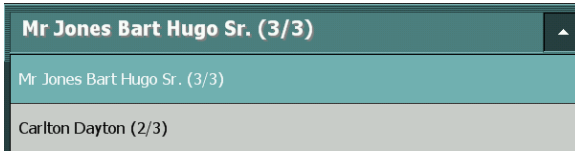

**Figure 159: NX – Examination environment Patient Switch with optionally configured image & exposure availability indication**

“# images available” refers to the amount of received images, and “# planned exposures” to the amount of exposures identified but for which no image was received yet from the Digitizer.

- Room (Central Monitoring System only)


The Patient Switch displays the name of the NX workstation where the exam is performed.



**Figure 160: NX – Examination environment Patient Switch with optionally configured room indication.**

- Combined Options

It is possible to combine multiple options, e.g. Patient Birth Date & Exam:

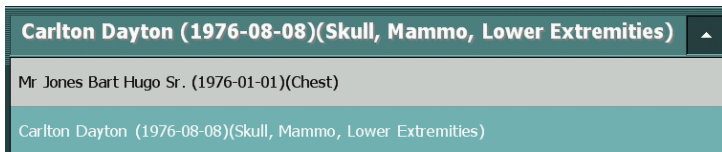

**Figure 161: NX – Examination environment Patient Switch with optionally configured patient birth date and exam indication**


## Related Links

[Person Name Representation](#) on page 208

[Regional Settings](#) on page 43

## Configuring External Applications

It is possible to configure additional NX action buttons, from which external applications can be launched or be brought to the foreground when already running.



**Figure 162: NX - Worklist Environment Action Buttons**



*Note: For Central Monitoring System it is not possible to configure an external application for the Worklist environment.*


To enable an action button for an NX environment:

1. Go to the General Settings section of the NX Service and Configuration Tool User Interface Configuration section.
2. Check the checkbox next to the preferred environment.
3. Supply a caption for the action button.

The supplied caption will be displayed on the button in NX.

4. Define the application linked with the action button.
5. To configure the application linked with the additional action button, the user can manually supply the path to the executable file or browse to the file by pressing the browse button.

It is also possible to configure a path pointing to a data file. When the additional action button is triggered in NX, the application associated with the file will be launched, opening the configured file.

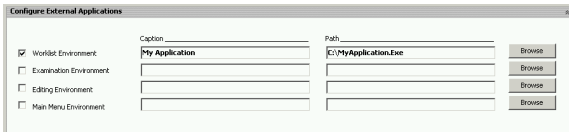

**Figure 163: NX Service and Configuration Tool – Enabled action button for the Worklist Environment**

6. Check the preview of the button that is available in the action button overview, by clicking on the NX environment link next to the checkbox. (This overview is not applicable for the Main Menu Environment).



**Figure 164: NX Service and Configuration Tool – Enabled action button for the Worklist Environment**




*Note: The presence of this action button can not be toggled from the action button overview pane.*



*Note: The order of the action buttons is fixed.*

- Click on the "Configure" button to navigate back to the "Configure External Applications" pane.

In NX the additional action button will be displayed as configured:

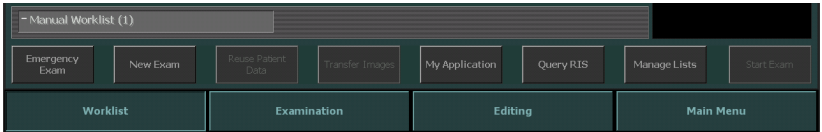

**Figure 165: NX– Additional Action Button**

## Worklist Settings

In the NX Service and Configuration Tool Worklist environment User Interface Settings section, the user can configure the look and feel of the NX Worklist Environment.

### Topics:

- [General Settings](#)
- [Worklist](#)
- [Closed Exams](#)
- [Search](#)

## General Settings

In the General Settings pane, the presence of the manual worklist and the action buttons can be configured for the NX Worklist environment.

### Topics:

- [Manual Worklist](#)
- [Action Buttons](#)

## Manual Worklist

By checking or un-checking the manual worklist checkbox, the presence of the manual worklist in the NX Worklist environment is toggled.



**Figure 166: NX Service and Configuration Tool – Manual Worklist configuration**

When the manual worklist option is enabled, the worklist will thus be present in the worklist environment.

Manual Worklist (1)				
Patient Name	Patient Identification	Birth Date	Age	Sex
Bart Hugo Jones	PatID12345	1/01/1976	26	Male

**Figure 167: NX– Manual Worklist**

It will further be possible to manage the manual worklist through the manage lists functionality:

**Manage Lists**

Manual Worklist    Worklist

**Browsing patient record 1 of 1**

Prefix :       Birth Date :  DD/MM/YYYY

First Name :       Age :

Middle Name :       Sex :

Last Name :

Suffix :

Patient Identification :

**Figure 168: NX– Manage Lists, Manual Worklist**

## Action Buttons

Within the Action Buttons section, the presence of the action buttons in the NX Worklist environment is toggled.

**Show Emergency Exam Button**

**Show New Exam Button**

**Show Reuse Patient Data Button**

**Show Manage Lists Button**

**Show Transfer Images Button**

**Show Query RIS Button**

**Show Start Exam Button**

**Show External Application Button**   

**Figure 169: NX Service and Configuration Tool – Action Buttons configuration**

The action buttons preview allows a visual inspection of the action buttons as they will be presented in NX.



**Figure 170: NX Service and Configuration Tool – Action Buttons preview**

From this preview the caption and order of the action buttons can be inspected.



*Note: The order of the actions buttons is fixed*

To enable the presence of an action button in an environment, it is sufficient to check the checkbox of the corresponding action button.

When an action button is enabled, it will be displayed in an enabled state (green) in the action button preview. If an action button is disabled, it will be displayed in a disabled state (white) in the action button preview.

The presence of some action buttons can not be toggled. Therefore the checkboxes to enable or disable these buttons are grayed out.

Action Button	Configurable	Rationale
Show Emergency Exam Button	Yes	
Show New Exam Button	No	It should always be possible to manually start an exam on an NX workstation. Therefore the presence of this action button is mandatory.
Show Reuse Patient Data Button	Yes	
Show Manage Lists Button	No	It should always be possible to manage either the worklist or the manual worklist. Therefore the presence of this action button is mandatory.
Show Transfer Images Button	Yes	
Show Query RIS Button	No	The presence of this button is determined by the presence of the RIS license. If no RIS license is present, the action button will not be enabled.
Show Start Exam Button	No	It should always be possible to start an exam (RIS exam or manual exam) from the worklist environment.


Show External Application Button	No	The presence of this action button is determined by the configuration in the “Configure External Applications” pane. Refer to “Configuring External Applications” .
----------------------------------	----	---

**Related Links**

[Configuring External Applications](#) on page 212

## Worklist

In the Worklist pane, the worklist layout can be configured for the NX Worklist environment.

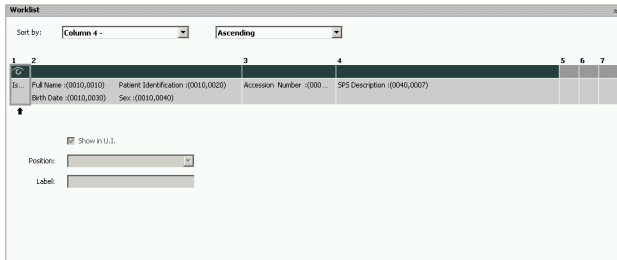

**Figure 171: NX Service and Configuration Tool – Configure Worklist**

Open Session Indicator	Patient Name	Accession Number	SPS Description
	Moambe Serge K4567 Male	ERR001	
	Baccilleri Bobby... K4567 Male	MOB12377	Abdomen AP
	Van Den Durpel... 2/08/1974 0:00:00 M11313 Female	GOR7111	Ankle AP
	Dupont Tony 11/09/1922 0:00:00 MOB4568 Female	JC6262	Cervical Spine AP
	Sellie Peter 12/11/2002 0:00:00 S789654 Male	GRO38	Clavicle AP
	Jos De 11/09/1922 0:00:00 JO3171 Female	TMF2555	Full Leg AP
	Teresa Black 11/09/1922 0:00:00 M5656 Female	TE1334	Chest AP
	Jones Bart 7/08/1981 0:00:00 OP78954 Female	FOP78954	Hand AP
	Smith George 5/08/1958 0:00:00 SSA0001 Male	US0001	Knee AP
	Emergency Patient 11/09/1922 0:00:00 Q50000 Female	WCK78643	Lumbar Spine

**Figure 172: NX– Worklist**

### Topics:

- [Content](#)
- [Sorting](#)

### Content

The first column (“Open Session Indicator”) is fixed. Neither the content nor the visibility can be toggled for this column.

For the six other columns the content can be defined by the user.

Per column, it is possible to configure up to four attributes for display:

2

Patient Name	
Full Name :(0010,0010)	Patient Identification :(0010,0020)
Birth Date :(0010,0030)	Sex :(0010,0040)

↑

**Figure 173: NX Service and Configuration Tool – Configure column contents**

Show in U.I.

Position:

Label:

Content:

Sort by:

**Figure 174: NX Service and Configuration Tool – Configure column contents**

The visibility of the column is toggled by checking or un-checking the checkbox. This extra visibility toggle allows easier customization of imported default configurations by making not desired columns invisible.

Column positions can be easily switched by selecting another position from the position drop-down box. The contents of the cells will be swapped.

A column label can be supplied.

Since a single entry in a column can contain up to four attributes, a sorting field must be assigned for when the column is sorted (ascending or descending). This is done by selecting one of the four selected attributes in the “Sort By” column.

## Sorting


For the whole worklist, the default sorting column and mode can be configured by selecting the desired values from the drop-down box.

Sort by:

The worklist will be sorted by the column defined in the “Sort By” drop-down box, in the configured mode.

## Closed Exams

In the Closed Exams pane, the closed exams list layout can be configured for the NX Worklist environment.

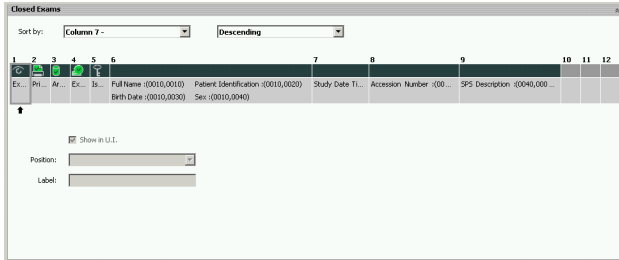

**Figure 175: NX Service and Configuration Tool – Configure Closed Exams List**

The screenshot shows the 'Closed Exams (5)' worklist table. The table has the following columns: 'Name', 'Study Date...', 'Accession Number', and 'SPS Description'. The rows contain the following data:

Name	Study Date...	Accession Number	SPS Description
test test	2007-12-...		
Carlton Dayton 1976-08-08... Male	2007-12-...		
gspjgiew	2007-12-...		
test	2007-12-...		
Billy Wayne 1976-10-10... Male	2007-12-...		

**Figure 176: NX– Worklist**

### Topics:

- [Content](#)
- [Sorting](#)

### Content

The first six columns:

- Open Session Indicator
- Print Automation
- Archive Automation
- Export Automation


- Dose Structured Report Export Automation Status
- Lock Sessions

are fixed. Neither the content nor the visibility can be toggled for these columns.


The automation columns are only visible if the automation functionality is enabled.

For the seven other columns the content can be defined by the user.

Per column, it is possible to configure up to four attributes for display:

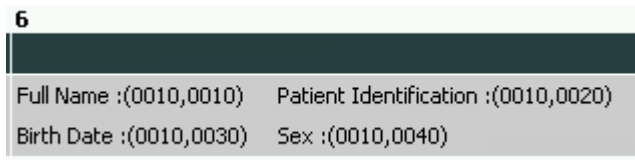

**Figure 177: NX Service and Configuration Tool – Configure column contents**

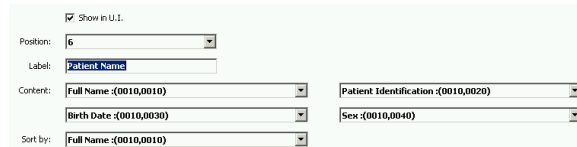

**Figure 178: NX Service and Configuration Tool – Configure column contents**

The visibility of the column is toggled by checking or un-checking the checkbox. This extra visibility toggle allows easier customization of imported default configurations by making not desired columns invisible.

Column positions can be easily switched by selecting another position from the position drop-down box. The contents of the cells will be swapped.

A column label can be supplied.

Since a single entry in a column can contain up to four attributes, a sorting field must be assigned for when the column is sorted (ascending or descending). This is done by selecting one of the four selected attributes in the “Sort By” column.

## Sorting

For the whole Closed Exams list, the default sorting column and mode can be configured by selecting the desired values from the drop-down box.



The Closed Exams list will be sorted by the column defined in the “Sort By” drop-down box, in the configured mode.

## Search

(Central Monitoring System Only!)

In the Search pane, the search list layout can be configured for the CMS NX Worklist environment.

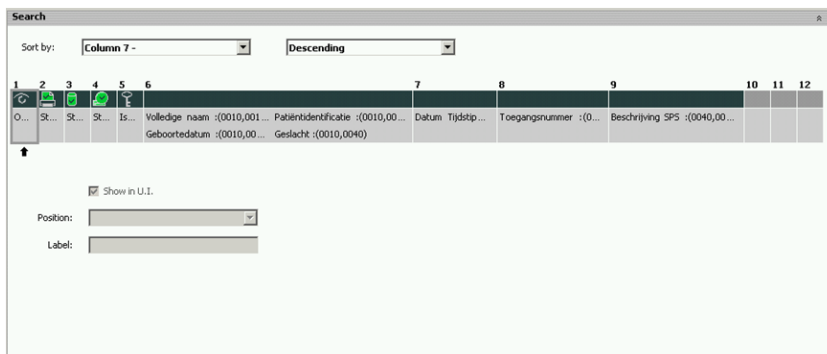


Figure 179: NX Service & Configuration Tool – Configure CMS Search List.

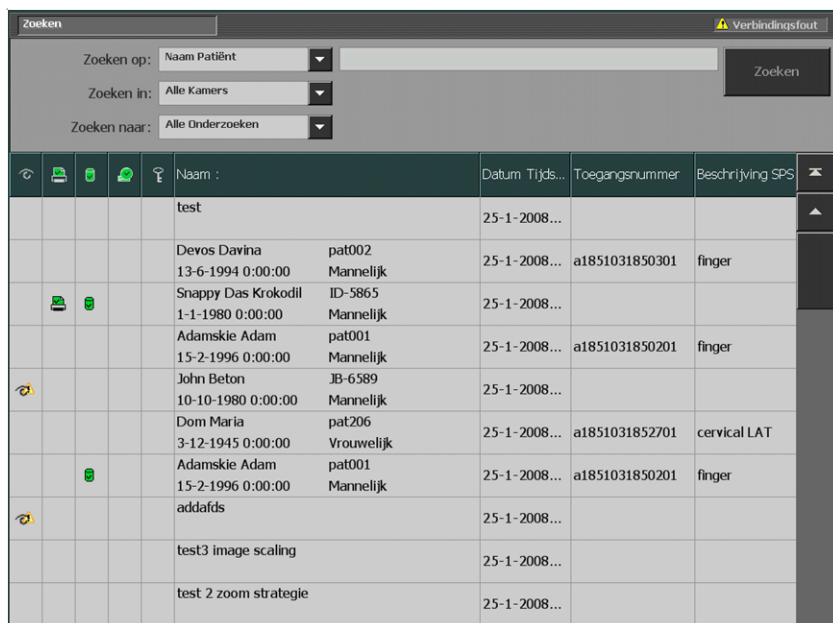


Figure 180: NX– Search list

### Topics:

- [Content](#)

- *Sorting*

## Content

The first column, Open Session Indicator, is fixed. Neither the content nor the visibility can be toggled for this column.

For the following four columns the visibility can be toggled.

- Print Automation
- Archive Automation
- Export Automation
- Lock Sessions

For the seven other columns the content can be defined by the user.

Per column, it is possible to configure up to four attributes for display:

6
Full Name :(0010,0010) Patient Identification :(0010,0020)
Birth Date :(0010,0030) Sex :(0010,0040)

**Figure 181: NX Service & Configuration Tool – Configure column contents**

<input checked="" type="checkbox"/> Show in U.I.	
Position:	6
Label:	Patient Name
Content:	Full Name :(0010,0010) Patient Identification :(0010,0020)
	Birth Date :(0010,0030) Sex :(0010,0040)
Sort by:	Full Name :(0010,0010)

**Figure 182: NX Service & Configuration Tool – Configure column contents**

The visibility of the column is toggled by checking or un-checking the checkbox. This extra visibility toggle allows easier customization of imported default configurations by making not desired columns invisible.

Column positions can be easily switched by selecting another position from the position drop-down box. The contents of the cells will be swapped.

A column label can be supplied.

Since a single entry in a column can contain up to four attributes, a sorting field must be assigned for when the column is sorted (ascending or descending). This is done by selecting one of the four selected attributes in the “Sort By” column.

## Sorting

For the whole Search list, the default sorting column and mode can be configured by selecting the desired values from the drop-down box.



**Figure 183: Default Sorting Column**

The Search list will be sorted by the column defined in the “Sort By” dropdown box, in the configured mode.

## Examination Settings

---

In the NX Service and Configuration Tool Examination environment User Interface Settings section, the user can configure the look and feel of the NX Examination Environment.


### Topics:

- [General Settings](#)
- [XRG Parameters](#)
- [View Patient](#)
- [Edit Patient](#)
- [View Image Details](#)
- [Edit Image Details](#)
- [Compose Exam](#)
- [Tools & Annotations](#)

## General Settings

In the General Settings pane, the presence of the action buttons can be configured for the NX Examination environment.

Within the Action Buttons section, the presence of the action buttons in the NX Examination environment is toggled.

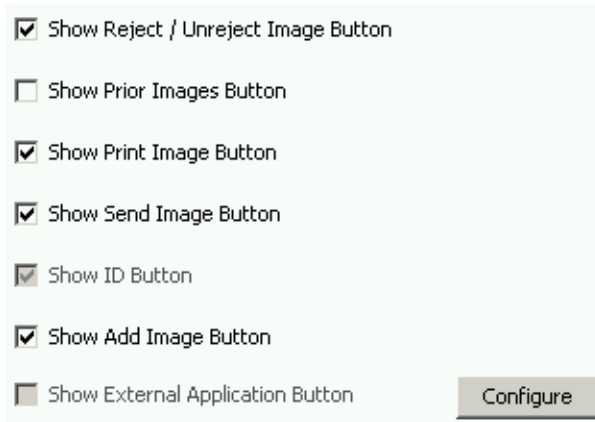

**Figure 184: NX Service and Configuration Tool – Action Buttons configuration**

The action buttons preview allows a visual inspection of the action buttons as they will be presented in NX.



**Figure 185: NX Service and Configuration Tool – Action Buttons preview**

From this preview the caption and order of the action buttons can be inspected.



*Note: The order of the actions buttons is fixed.*

To enable the presence of an action button in an environment, it is sufficient to check the checkbox of the corresponding action button.


When an action button is enabled, it will be displayed in an enabled state (green) in the action button preview. If an action button is disabled, it will be displayed in a disabled state (white) in the action button preview.

The presence of some action buttons can not be toggled. Therefore the checkboxes to enable or disable these buttons are grayed out.


Action Button	Configurable	Rationale
Show Reject/Unreject Image Button	Yes	
Show Prior Images Button	Yes	
Show Print Image Button	Yes	
Show Send Image Button	Yes	
Show ID Button	No	It should always be possible to identify an exposure, therefore the presence of this action button is mandatory.
Show Add Image Button	Yes	
Show External Application Button	No	The presence of this action button is determined by the configuration in the “Configure External Applications” pane.

## XRG Parameters

Within the XRG Parameters pane, the layout of the XRG pane in the NX Examination environment can be configured.

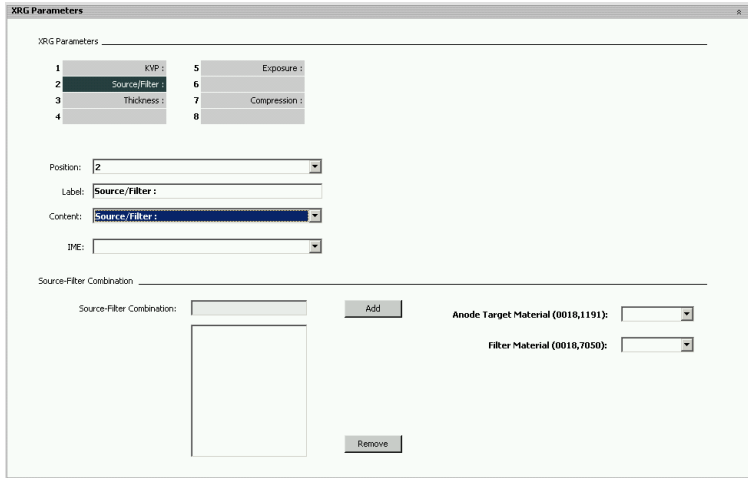


**Figure 186: NX Service and Configuration Tool – Configure XRG Parameters**



**Figure 187: NX– Examination XRG Parameters**

Up to eight attributes can be configured for display.

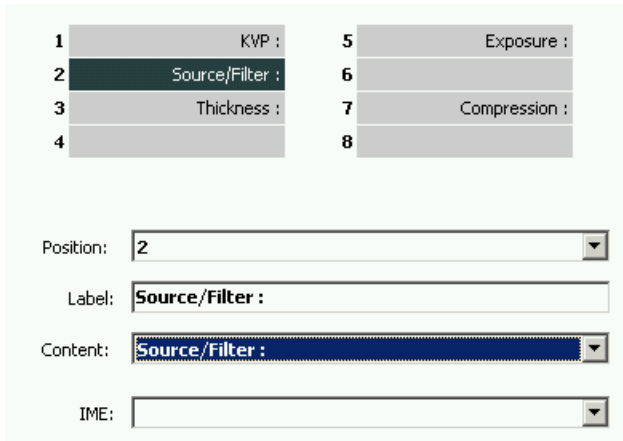


**Figure 188: NX Service and Configuration Tool – Configure XRG Parameters**

To configure an attribute, an entry is selected from the “Content” drop-down box after having selected a target field. This can be done by clicking on a field in the overview, or by selecting a field from the “Position” drop-down box.

After having selected an attribute from the “Content” drop-down box, a custom label can be provided next to the default presented label.

Configured attributes positions can be easily switched by selecting another position from the position drop-down box. The contents of the positions will be swapped.


In case of run-time user editable fields, the IME (Input Method Editor) can also be defined.

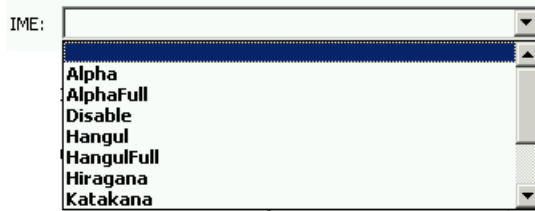

**Figure 189: NX Service and Configuration Tool – IME selection drop-down box**

The IME selection is dependent of the DICOM character set configuration in the Workstation Settings.

For the attribute “Source/Filter”, an additional configuration section is available.

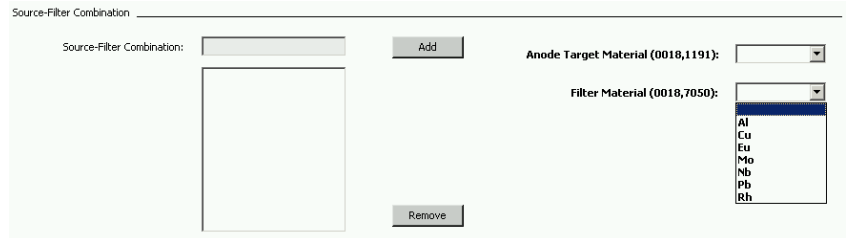

**Figure 190: NX Service and Configuration Tool – Source-Filter Combination configuration**

Within the Source-Filter configuration section, the values presented in the Source-Filter drop-down in NX can be configured.

The list of Source-Filter combinations is populated by selection a value for the DICOM attribute “Anode Target Material”, followed by selecting a value for the DICOM attribute “Filter Material”. The selection should be confirmed by pressing the “Add” button.

By pressing the “Remove” button, a selected Source-Filter combination can be deleted.

## Related Links


[Workstation General Settings](#) on page 40

## View Patient

Within the View Patient pane, the layout of the View Patient Details pane in the NX Examination environment can be configured.



**Figure 191: NX Service and Configuration Tool – Configure View Patient pane**



**Figure 192: NX – Patient pane**

Up to eight attributes can be configured for display.


To configure an attribute, an entry is selected from the “Content” drop-down box after having selected a target field. This can be done by clicking on a field in the overview, or by selecting a field from the “Position” drop-down box.

After having selected an attribute from the “Content” drop-down box, a custom label can be provided next to the default presented label.


Configured attributes positions can be easily switched by selecting another position from the position drop-down box. The contents of the positions will be swapped.

## Edit Patient

Within the Edit Patient pane, the layout of the Edit Patient Details pane in the NX Examination environment can be configured.

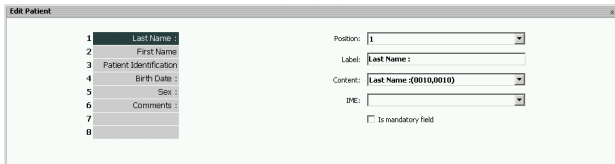

**Figure 193: NX Service and Configuration Tool – Configure Edit Patient pane**

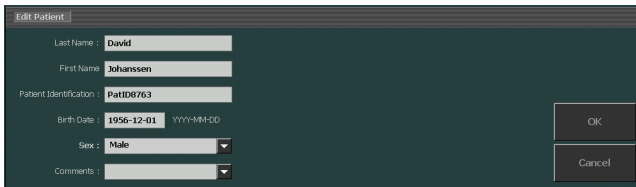

**Figure 194: NX – Edit Patient pane**

Up to eight attributes can be configured for editing.

To configure an attribute, an entry is selected from the “Content” drop-down box after having selected a target field. This can be done by clicking on a field in the overview, or by selecting a field from the “Position” drop-down box.

After having selected an attribute from the “Content” drop-down box, a custom label can be provided next to the default presented label.


For every configured attribute the “Is Mandatory” checkbox can be checked optionally. This action makes providing a value for the attribute mandatory in NX. In NX, mandatory fields are indicated by an asterisk (\*) next to the field.



**Figure 195: NX – Edit Patient pane, mandatory fields**

Configured attributes positions can be easily switched by selecting another position from the position drop-down box. The contents of the positions will be swapped.

In case of run-time user editable fields, the IME (Input Method Editor) can also be defined.

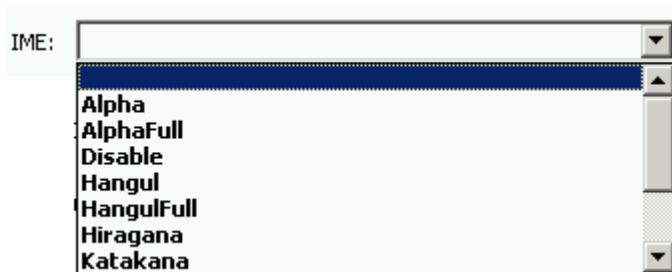

**Figure 196: NX Service and Configuration Tool – IME selection drop-down box**


The IME selection is dependent of the DICOM character set configuration in the Workstation Settings.

#### **Related Links**

[Workstation General Settings](#) on page 40

## View Image Details

Within the View Image Details pane, the layout of the View Image Details pane in the NX Examination environment can be configured.

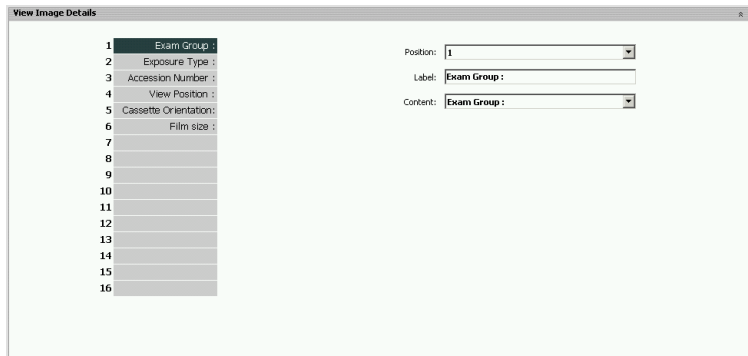

**Figure 197: NX Service and Configuration Tool – Configure View Image Details pane**



**Figure 198: NX – Image Details pane**

Up to 16 attributes can be configured for display.


To configure an attribute, an entry is selected from the “Content” drop-down box after having selected a target field. This can be done by clicking on a field in the overview, or by selecting a field from the “Position” drop-down box.

After having selected an attribute from the “Content” drop-down box, a custom label can be provided next to the default presented label.


Configured attributes positions can be easily switched by selecting another position from the position drop-down box. The contents of the positions will be swapped.

## Edit Image Details

Within the Edit Image Details pane, the layout of the Edit Image Details pane in the NX Examination environment can be configured.

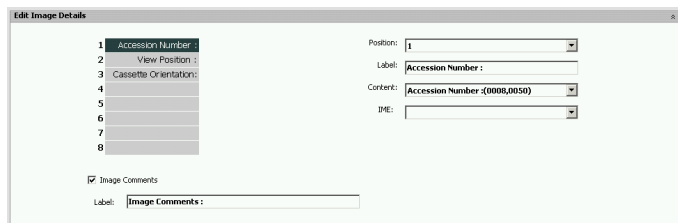

**Figure 199: NX Service and Configuration Tool – Configure Edit Image Details pane**

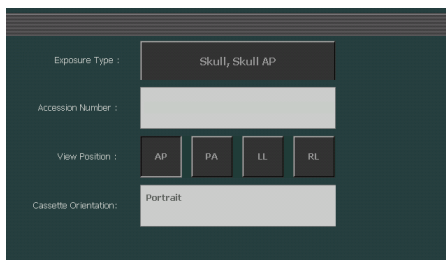

**Figure 200: NX– Image Details pane**


Up to eight attributes can be configured for editing.

To configure an attribute, an entry is selected from the “Content” drop-down box after having selected a target field. This can be done by clicking on a field in the overview, or by selecting a field from the “Position” drop-down box.

After having selected an attribute from the “Content” drop-down box, a custom label can be provided next to the default presented label.

Configured attributes positions can be easily switched by selecting another position from the position drop-down box. The contents of the positions will be swapped.

In case of run-time user editable fields, the IME (Input Method Editor) can also be defined.

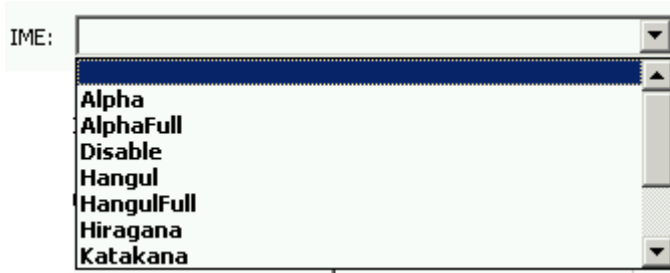

**Figure 201: NX Service and Configuration Tool – IME selection drop-down box**


The IME selection is dependent of the DICOM character set configuration in the Workstation Settings.

For the attribute “Image Comments”, an additional configuration element is available. To make the image comments, configured in the General Configuration section Predefined Lists, available in NX, the checkbox must be checked.

A user defined label can additionally be supplied.



**Figure 202: NX Service and Configuration Tool – Image Comment attribute configuration**

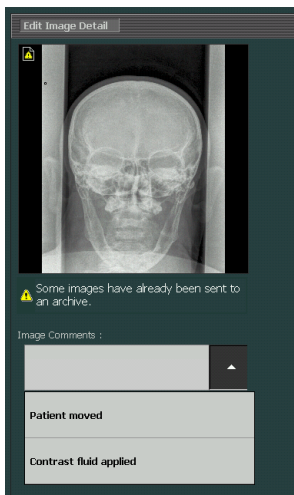

**Figure 203: NX – Image Comment attribute in the Edit Image Details pane**


## Related Links

[Workstation General Settings](#) on page 40

[Predefined Lists](#) on page 46

## Compose Exam

Within the Compose Exam pane, the layout of the Add Image pane in the NX Examination environment can be configured.

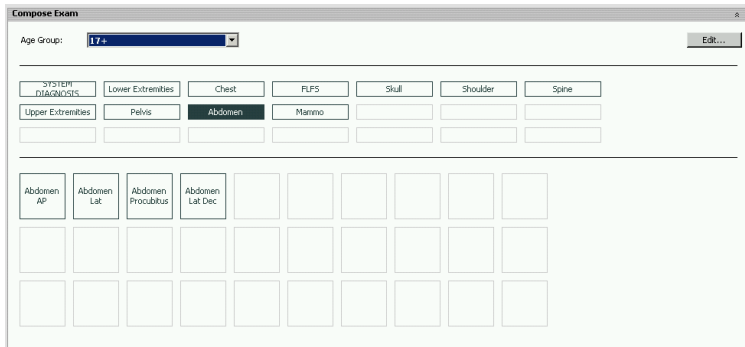

**Figure 204: NX Service and Configuration Tool – Compose Exam pane**



**Figure 205: NX– Add Image pane**

The availability of items in the Compose Exam pane is dependent of some factors:

- When no pediatric license is enabled, the “Age Group” drop-down box will only contain the adult age group.
- When an exam or exposure type does not have its visibility flag enabled, it will not be available in the Compose Exam pane.

As a shortcut, the “Edit...” button provides quick access to the Exam Tree.

To define the layout of the Add Image pane, the exam and exposure type/group buttons can be dragged and dropped to the desired location. The available exposure types/groups depend on the selected exam group.


When a location is unavailable, the position will be indicated in grey.

**Related Links**

[Configuring Examination Groups](#) on page 160

## Tools & Annotations

Within the Tools & Annotations pane, the layout of the NX Examination environment toolbox can be configured.

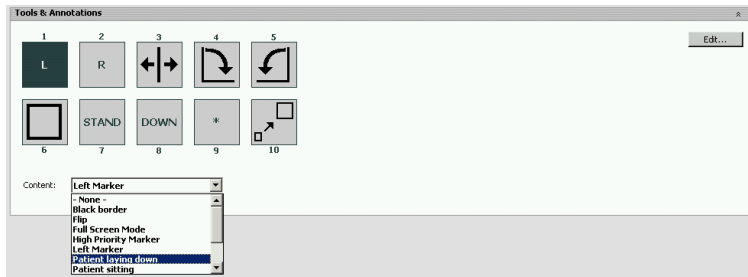

**Figure 206: NX Service and Configuration Tool – Tools & Annotations pane**



**Figure 207: NX– Examination environment Toolbox**

Up to ten Tools can be selected from the “Contents” drop-down box.

The “Contents” drop-down box is populated by the configured Custom Markers. The “Edit...” button allows quick access to this configuration section.

Additionally the following Tools are available:

- Black Border
- Flip
- Full Screen Mode
- Rotate clockwise
- Rotate counter clockwise
- Freehand rotate

It is also possible not to configure a specific button by selecting the entry “-None -” from the content drop-down box.

## Editing Settings

In the NX Service and Configuration Tool Editing environment User Interface Settings section, the user can configure the look and feel of the NX Editing Environment.

### Topics:

- [General Settings](#)

- *Softcopy & Print View*
- *Tools & Annotations*

## General Settings

In the General Settings pane, the Editing environment view mode options and action buttons can be configured for the NX Editing environment.

### Topics:

- [View Mode](#)
- [Action Buttons](#)

### View Mode

The NX Editing environment consists of two view modes:

- Softcopy View
- Print View




**Figure 208: NX Service and Configuration Tool – View Mode options**

The default view mode of the Editing environment can be configured by selecting the corresponding option:

Caption	Function
Show images by default in normal mode	The first time an image is viewed in the NX Editing environment, it will be displayed by default in the Softcopy View mode.
Show images by default in print mode	The first time an image is viewed in the NX Editing environment, it will be displayed by default in the Print View mode.

In case the system will be used in one view mode exclusively, it is not necessary to be able to switch between view modi. For this situation, the possibility is offered to disable the presence of the view mode toggle button:

Caption	Function
Show Normal Mode/Print Mode Toggle Button = ON	The view mode toggle button is displayed in the NX Editing Environment:

	
Show Normal Mode/Print Mode Toggle Button = OFF	The view mode toggle button is not displayed in the NX Editing Environment.

The NX Editing environment can be configured for use with touch screen. This affects the behaviour of the left toolbar and the button functions.

Caption	Function
Enable touch mode	This affects the behaviour of the left toolbar and the button functions.



*Note:* Depending on the configuration, this option may be unavailable and touch mode may be enabled by default.


## Action Buttons

Within the Action Buttons section, the presence of the action buttons in the NX Editing environment is toggled.

- Show Reject / Unreject Image Button
  - Show CATH Button
  - Show Save as New Button
  - Show Print Sheet Button
  - Show Send Image Button
  - Show Close And Send All Button
  - Show External Application Button
- [Configure](#)

**Figure 209: NX Service and Configuration Tool – Action Buttons configuration**

The action buttons preview allows a visual inspection of the action buttons as they will be presented in NX.



**Figure 210: NX Service and Configuration Tool – Action Buttons preview**

From this preview the caption and order of the action buttons can be inspected.

To enable the presence of an action button in an environment, it is sufficient to check the checkbox of the corresponding action button.

When an action button is enabled, it will be displayed in an enabled state (green) in the action button preview. If an action button is disabled, it will be displayed in a disabled state (white) in the action button preview.

The presence of some action buttons can not be toggled. Therefore the checkboxes to enable or disable these buttons are grayed out.

Action Button	Configurable	Rationale
Show Reject/Unreject Image Button	Yes	
Show CATH Button	Yes	
Show Save as New Button	Yes	
Show Print Button	Yes	
Show Send Image Button	Yes	
Show Send Image Button	Yes	
Show External Application Button	No	The presence of this action button is determined by the configuration in the “Configure External Applications” pane.

## Softcopy & Print View


In the Softcopy & Print View pane, the presence of the true scale factor and the Status Box can be configured for the NX Editing environment.

### Topics:

- *True Scale factor*
- *Status Box*


### True Scale factor

When an image is viewed in Print View mode in the NX Editing environment, it is possible to display the scaling factor.



**Figure 211: NX Service and Configuration Tool – True Scale factor configuration**

When the option “Show true scale factor (print view)” is enabled, the scale factor of the image can be inspected in the NX Editing environment Status Box.



**Figure 212: NX– True Scale factor indication**

The scale factor can be divided in three main types:

- True size: When the scaling factor of an image is set to “True Size”, the displayed true scale factor will be “100%”.
- Best Fit: When the scaling factor of an image is set to “Best Fit”, the displayed true scale factor will be equal to the scaling factor applied to the image.
- Calibrated scale factor: When the calibration tool has been used for calibrating a distance measurement, a calibration indication (“CAL”) will be displayed next to the true sale factor.

Scale Mode	Best Fit	True Size	Calibrated
Example			

## Status Box

In the Status Box configuration section, the contents of the NX Status Box can be configured. The status box is displayed in both view modi of the NX Editing environment. The Status Box configuration applies to both NX View modi.

Status Box

Label:

Content:

Label:

Content:

Label:

Content:

**Figure 213: NX Service and Configuration Tool – Status Box configuration**

The Status Box can display up to four parameters. The available parameters are:

- Window Width (0028,1051)
- Window Centre (0028,1050)
- LGM (0018,1405)
- EI
- DI

For every parameter, a user-defined label can be provided which will be used for display in the NX Status Box:

Status Box Configuration	NX Status Box
	<pre>Level : 50 Window: 50 LgM : 1,36</pre>

Status Box	
Label:	<b>Level :</b>
Content:	<b>L :(0028,1050)</b>
Label:	<b>Window:</b>
Content:	<b>W :(0028,1051)</b>
Label:	<b>LgM :</b>
Content:	<b>LGM :(0018,1405)</b>

## Tools & Annotations

In the Tools & Annotations pane, the available NX Editing environment (annotation) tools can be configured.

For every available (annotation) tool, the presence of the corresponding button can be toggled by checking or un-checking the corresponding checkbox.


### Related Links



[Custom Markers](#) on page 48

### Topics:



- [Selection Palette](#)
- [Annotations Palette](#)
- [Transformation Palette](#)
- [View Palette](#)
- [Image Processing Palette](#)



### Selection Palette




Item	NX Control	Remark
Delete		The button is enabled in the NX Editing environment when an annotation is selected.








Select		The select function can be used to exit a selected annotation function and to return to selection mode.
Revert to Original		The “Revert to Original” functionality is used to undo all changes applied to the image using the Tools & Annotations pane.









## Annotations Palette


Item	NX Control	Remark
Left Marker		<p>When the “Left Marker” checkbox is checked, the Left Marker functionality will be available as a separate button in the NX Editing environment toolbox.</p> <p>The left marker is also available as a custom marker within the Custom Markers drop-down box.</p>
Right Marker		<p>When the “Right Marker” checkbox is checked, the Right Marker functionality will be available as a separate button in the NX Editing environment toolbox.</p> <p>The right marker is also available as a custom marker within the Custom Markers drop-down box.</p>
Custom Marker		<p>When the “Custom Markers” checkbox is checked, the defined custom markers will be displayed in the a drop-down box.</p> <p>The custom markers are defined in the “Custom Markers” pane of the General Settings section:</p>

		<table border="1"> <thead> <tr> <th>Name</th> <th>Text</th> <th>Functionality</th> <th>Size</th> </tr> </thead> <tbody> <tr> <td>L</td> <td>L</td> <td>Left</td> <td>10</td> </tr> <tr> <td>R</td> <td>R</td> <td>Right</td> <td>10</td> </tr> <tr> <td>HPM</td> <td>*</td> <td>High priority</td> <td>10</td> </tr> <tr> <td>SIT</td> <td>Patient sitting</td> <td></td> <td>10</td> </tr> <tr> <td>DOWN</td> <td>Patient laying down</td> <td></td> <td>10</td> </tr> <tr> <td>STAND</td> <td>Patient standing</td> <td></td> <td>10</td> </tr> <tr> <td></td> <td>[add a new marker]</td> <td></td> <td></td> </tr> <tr> <td></td> <td>[add a new marker]</td> <td></td> <td></td> </tr> <tr> <td></td> <td>[add a new marker]</td> <td></td> <td></td> </tr> <tr> <td></td> <td>[add a new marker]</td> <td></td> <td></td> </tr> <tr> <td></td> <td>[add a new marker]</td> <td></td> <td></td> </tr> <tr> <td></td> <td>[add a new marker]</td> <td></td> <td></td> </tr> </tbody> </table>	Name	Text	Functionality	Size	L	L	Left	10	R	R	Right	10	HPM	*	High priority	10	SIT	Patient sitting		10	DOWN	Patient laying down		10	STAND	Patient standing		10		[add a new marker]				[add a new marker]				[add a new marker]				[add a new marker]				[add a new marker]				[add a new marker]		
Name	Text	Functionality	Size																																																			
L	L	Left	10																																																			
R	R	Right	10																																																			
HPM	*	High priority	10																																																			
SIT	Patient sitting		10																																																			
DOWN	Patient laying down		10																																																			
STAND	Patient standing		10																																																			
	[add a new marker]																																																					
	[add a new marker]																																																					
	[add a new marker]																																																					
	[add a new marker]																																																					
	[add a new marker]																																																					
	[add a new marker]																																																					
<p>Free Text</p>		<p>When the “Free Text” checkbox is checked, it will be possible to add a free text annotation to an image.</p> <p>The default size of the free text annotation can be set in the “Image Presentation” pane of the Workflow Management section:</p> <p>Free Text font size: <input type="text" value="10"/></p>																																																				
<p>Predefined Text</p>		<p>When the “Predefined Text” checkbox is checked, it will be possible to add a predefined text annotation to an image.</p> <p>The predefined text annotations can be set in the “Predefined lists” pane of the General Settings section:</p> <p>Predefined Texts</p> <p>Predefined Texts: <input type="text"/> <input type="button" value="Add"/></p> <p>Font Size (mm): <input type="text" value="10"/></p> <ul style="list-style-type: none"> <li>After 5 minutes</li> <li>After 10 minutes</li> <li>After 15 minutes</li> <li>After 30 minutes</li> <li>After 1 hour</li> <li>After 2 hours</li> <li>Oral contrast</li> <li>IV contrast</li> <li>IA contrast</li> <li>With zoru granules</li> <li>Tomo distance 75</li> <li>Tomo distance 100</li> </ul> <p><input type="button" value="Up"/> <input type="button" value="Down"/> <input type="button" value="Remove"/></p>																																																				





		
Arrow		<p>When the “Arrow” checkbox is checked, it will be possible to add an arrow annotation to an image.</p> <p>When adding an arrow annotation to an image, it will also be possible to add a custom text annotation.</p>
Rectangle		<p>When the “Rectangle” checkbox is checked, it will be possible to add a rectangle annotation to an image.</p> <p>When adding a rectangle annotation to an image, an area measurement will be displayed along.</p>


Circle		<p>When the “Circle” checkbox is checked, it will be possible to add a circle annotation to an image.</p> <p>When adding a circle annotation to an image, an area and diameter measurement will be displayed along.</p>
Polygon		<p>When the “Polygon” checkbox is checked, it will be possible to add a polygon annotation to an image.</p> <p>When adding a polygon annotation to an image, an area measurement will be displayed along.</p>
Freehand		<p>When the “Freehand” checkbox is checked, it will be possible to add a freehand annotation to an image.</p> <p>When adding a freehand annotation to an image, an area measurement will be displayed along.</p>
Perpendicular		<p>When the “Perpendicular” checkbox is checked, it will be possible to add a perpendicular annotation to an image.</p>
Line		<p>When the “Line” checkbox is checked, it will be possible to add a line annotation to an image.</p>
Rectangle SAL		<p>When the “Rectangle SAL” checkbox is checked, it will be possible to perform a SAL (Scan Average Level) measurement on an image.</p>
Rectangle PVI		<p>When the “Rectangle PVI” checkbox is checked, it will be possible to perform a PVI (Pixel Value Index) measurement on an image.</p>

Rectangle EI		When the “Rectangle EI” checkbox is checked, it will be possible to perform an EI (Exposure Index) measurement on an image.
Calibrate a line		When the “Calibrate a line” checkbox is checked, it will be possible to perform a line calibration.
Calibrate a circle		When the “Calibrate a circle” checkbox is checked, it will be possible to perform a circle calibration.
ERMF calibration		When the “ERMF calibration” checkbox is checked, it will be possible to perform an Estimated Radiographic Magnification Factor (ERMF) calibration.
Measure an angle		When the “Measure an angle” checkbox is checked, it will be possible to perform an angle measurement.
Measure a distance		When the “Measure a distance” checkbox is checked, it will be possible to perform a distance measurement.
Measure a leg difference		When the “Measure a leg difference” checkbox is checked, it will be possible to perform a leg difference measurement.
Measure scoliosis		When the “Measure scoliosis” checkbox is checked, it will be possible to perform a scoliosis measurement.
Annotation Color		When the “Annotation Color” checkbox is checked, it will be possible to set the color for a selected annotation.





		<p>The operator selects an annotation on the image and afterwards a color from the Annotation Color drop-down box to set the color of an annotation.</p>
--	---	--


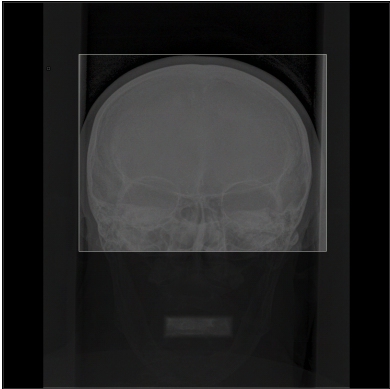


## Transformation Palette

Item	NX Control	Remark
Rotate Clockwise		<p>The button is present in the NX Editing environment when the checkbox is enabled in the Transformation Palette.</p> <p>The “Rotate Clockwise” functionality is used to rotate an image clockwise.</p>
Rotate Counter Clockwise		<p>The button is present in the NX Editing environment when the checkbox is enabled in the Transformation Palette.</p> <p>The “Rotate Counter Clockwise” functionality is used to rotate an image counter clockwise.</p>
Freehand Rotate		<p>The button is present in the NX Editing environment when the checkbox is enabled in the Transformation Palette.</p> <p>The “Freehand Rotate” functionality is used to rotate an image by an arbitrary angle.</p>
Flip		<p>The button is present in the NX Editing environment when the checkbox is enabled in the Transformation Palette.</p> <p>The “Flip” functionality is used to flip an image over the vertical axis.</p>


Show/Hide Square Marker		<p>The button is present in the NX Editing environment when the checkbox is enabled in the Transformation Palette.</p> <p>The “Show/Hide Square Marker” functionality is used to toggle the presence of the Square Marker.</p>
-------------------------	---	--








## View Palette







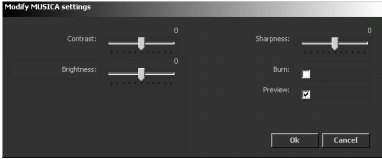
Item	NX Control	Remark
Zoom In		<p>When the “Zoom In” checkbox is checked, it will be possible to zoom in on a viewed image.</p> <p>When the button is not checked, and thus not present in NX, it is still possible to perform zoom actions with the context menu and mouse scroll wheel.</p>
Zoom Out		<p>When the “Zoom Out” checkbox is checked, it will be possible to zoom out on a viewed image.</p> <p>When the button is not checked, and thus not present in NX, it is still possible to perform zoom actions with the context menu and mouse scroll wheel.</p>
Zoom to ROI		<p>When the “Zoom to ROI” checkbox is checked, it will be possible to zoom in to a specific region of interest on the image.</p> <p>The region of interest must be indicated on the image before the zoom is actually performed.</p>
Reset Zoom		<p>When the “Reset Zoom” checkbox is checked, it will be possible to reset the zoom factor to its original state.</p> <p>This function is only applicable for images on which zoom actions (zoom in and/or zoom out) have been performed.</p>

Enable/ disable Shutters		<p>When the “Enable/disable Shutters” checkbox is checked, it will be possible to apply manual shutters on an image:</p>  <p>When disabling the shutter function, the shuttered area will remain indicated, the shutter borders will however not be editable anymore.</p>
Enable/ disable split view		<p>When the “Enable/disable split view” checkbox is checked, it will be possible to toggle the split view mode of an image.</p>
Enable/ disable Full Screen		<p>When the “Enable/disable Full Screen” checkbox is checked, it will be possible to toggle the full screen view mode of an image.</p>

### Image Processing Palette

Item	NX Control	Remark
Window Level		<p>When the “Window Level” checkbox is checked, it will be possible to adjust the window and level settings of an image.</p>

Undo Window Level		When the “Undo Window Level” checkbox is checked, it will be possible to discard the window and level changes made to an image.
Musica		When the “Musica” checkbox is checked, it will be possible to display and use the interactive Musica dialog box:  
Collimation		When the “Collimation” checkbox is checked, it will be possible to perform collimation actions on the viewed image.  On DR images and CR 10/12-X images, the collimation area also defines the cropping area.
Collimation Rectangle		When the “Collimation Rectangle” checkbox is checked, it will be possible to draw rectangular collimation shapes on the viewed image.  On DR images and CR 10/12-X images, the collimation area also defines the cropping area.
Collimation Polygon		When the “Collimation Polygon” checkbox is checked, it will be possible to draw polygon collimation shapes on the viewed image.  On DR images and CR 10/12-X images, the collimation area also defines the cropping area.
Collimation Circle		When the “Collimation Circle” checkbox is checked, it will be possible to draw circular collimation shapes on the viewed image.

		On DR images and CR 10/12-X images, the collimation area also defines the cropping area.
Invert Collimation Area		When the “Invert Collimation Area” checkbox is checked, it will be possible to invert an indicated collimation area on the viewed image.
Collimation Border		When the “Collimation Border” checkbox is checked, it will be possible to toggle the collimation border of the viewed image.  On DR images and CR 10/12-X images, this tool turns on or off cropping of the non-relevant image area's.
Histogram		When the “Histogram” checkbox is checked, it will be possible to toggle the display of the image histogram:  
Burn		When the “Burn” checkbox is checked, it will be possible to toggle the burn of the viewed image.
Invert		When the “Invert” checkbox is checked, it will be possible to invert a viewed image.
Enable/Disable Background Darkening		When the “Enable/disable Background Darkening” checkbox is checked, it will be possible to toggle the background darkening of a mammo image.

**Figure 214: e.g. histogram for MUSICA image processing**



# Using the Offline NX Service and Configuration Tool

---

## Topics:

- *Introduction*
- *Prerequisites*
- *Limitations*
- *Licenses*
- *Using the offline NX Service and Configuration Tool*
- *Special: Configuring Bitmap Images to be Printed on Film*

## Introduction

---

The Offline NX Service and Configuration Tool is an auxiliary tool for the Field Service Engineer. The Field Service Engineer can load and configure any NX configuration file on the offline NX Service and Configuration Tool installed on a service PC. This enables the Field Service Engineer to prepare the configuration file before going to the site.

The offline NX Service and Configuration Tool provides basically the same functionalities as the online NX Service and Configuration Tool (= the one installed on a real NX system). There are some limitations though which are described in this document.

Every NX version starting from NX2.0.68XX will have its own version of the offline NX Service and Configuration Tool. The different versions can be installed next to one another (the version number is part of the name of the installation path: C:\Agfa\Healthcare\NX\Offline NX Service and Configuration Tool <Version>\Bin).

## Prerequisites

---

- Windows Vista SP2, Windows 7 SP1, Windows 8, Windows 8.1.
- Minimum screen resolution: 1024 x 768
- Local administrator rights on the PC on which you want to install and run the offline NX Service and Configuration Tool.

## Limitations

---

There is no access to the NX database. Input and output goes via export files (xml). These are the same type of files as used in the previous NX versions with the online NX Service and Configuration Tool. Activating, loading or restoring of the configuration is not possible.

Further:

- No license file required!
- No authentication configuration (users and roles): as this data is stored in a separate repository
- No test connection functionalities
- No query RIS
- No test image for the monitor check
- No scan for in-room NXs (CMS functionality)
- No delete session (as there is no NX DB)
- No automatic backup is foreseen

### Related Links

[Licenses](#) on page 262

## Licenses

---


The offline NX Service and Configuration Tool does not work with real licenses. All licenses are available without having to load an ALF file!

Therefore you must manually disable licenses in the 'Security and License management' pane in order to come as close as possible to the online NX situation. Remember that enabling\disabling licenses in the NX Service and Configuration Tool has a important impact on the GUI and verification logic in the NX Service and Configuration Tool!

## Using the offline NX Service and Configuration Tool

1. Start > Programs > Agfa > NX > Offline NX Service and Configuration Tool 3.0.XXXX > Start Offline NX Service and Configuration Tool XX.

The startup screen of the tool offers following possibilities:

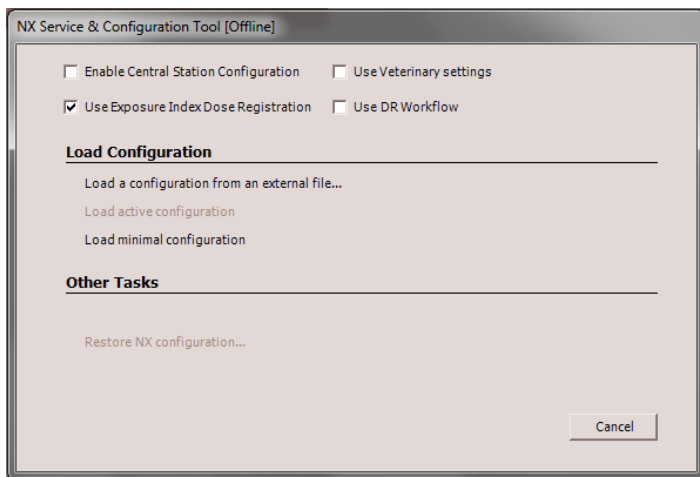

**Figure 215: Offline NX Service and Configuration Tool Startup dialog box.**

- **Enable Central Station Configuration:**  
You can make a distinction between configuring for a normal NX or a CMS NX.  
Check this box to configure a CMS. Only here this choice can be made!
- **Use Exposure Index Dose Registration**
- **Use Veterinary Settings**  
Check this box to configure a system with a veterinary license.
- **Use DR Workflow**  
This option is only enabled when the Exposure Index checkbox is checked.  
Check this box to edit a configuration for an NX Workstation that is connected to a DR Detector.
- **Select the software license edition:**  
Depending on the licenses available on the NX Workstation, the applicable version number must be selected.
- **Load configuration from an external file:**  
You can load an already existing configuration file in the NX Service and Configuration Tool. This can also be an export file made by an


online NX Service and Configuration Tool or a previous version of NX NX Service and Configuration Tool.

- Start creating a configuration from scratch by loading a minimal configuration.

The minimal configuration is different for non-CMS and CMS. This functionality is not available in the online NX Service and Configuration Tool. There, the NX database makes sure that a minimal configuration is always foreseen.

2. Set up the configuration as much as possible. Refer to “Limitations” .
3. Export the configuration to a file.

Before exporting, the configuration is automatically verified. When verification errors occur, one still has to option to save anyway (press <Continue>).

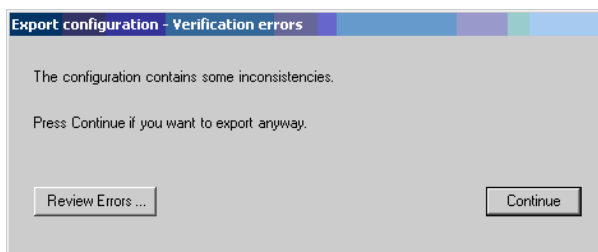

**Figure 216: Offline NX Service and Configuration Tool Startup dialog box - Verification dialog box.**


4. Import this export file in an online NX NX Service and Configuration Tool, finish the configuration and activate it.

## Related Links

[Limitations](#) on page 261

## Special: Configuring Bitmap Images to be Printed on Film

When configuring bitmaps to be printed on film, you can upload a bitmap file in the NX Service and Configuration Tool:

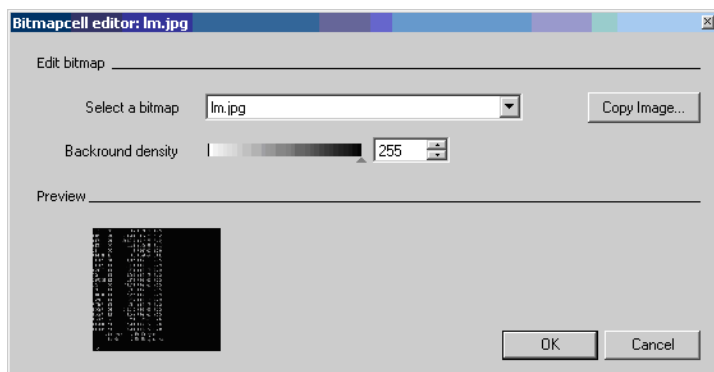

**Figure 217: Offline NX Service and Configuration Tool - bitmap cell editor.**

Clicking the button **Copy Image** will copy the file to a specific folder on the PC:

- On an offline NX Service and Configuration Tool system the bitmap file is copied to : C:\Agfa\Healthcare\NX\Offline.Config.Tool.XX\Bin\DataFiles\Configuration\BitmapFiles
- On an online NX Service and Configuration Tool, this directory is: C:\Agfa\Healthcare\NX\Configuration\BitmapFiles

When the configuration is activated on an online NX Workstation, you must manually copy the files from the offline BitmapFiles-folder to the BitmapFiles-folder on the NX Workstation.